


# MASS SPECTROMETRY REPORT

10-Mar-2017  
14:42:16

Probe: ESI  
Cone: 50v  
Desovation Temp: 350  
Capillary: 3.00KV  
Extractor: 5v  
Gas Flow: 350  
Scan ES+  
2.06e6

170310-31 1056 (19.518) Cm (1056:1057)

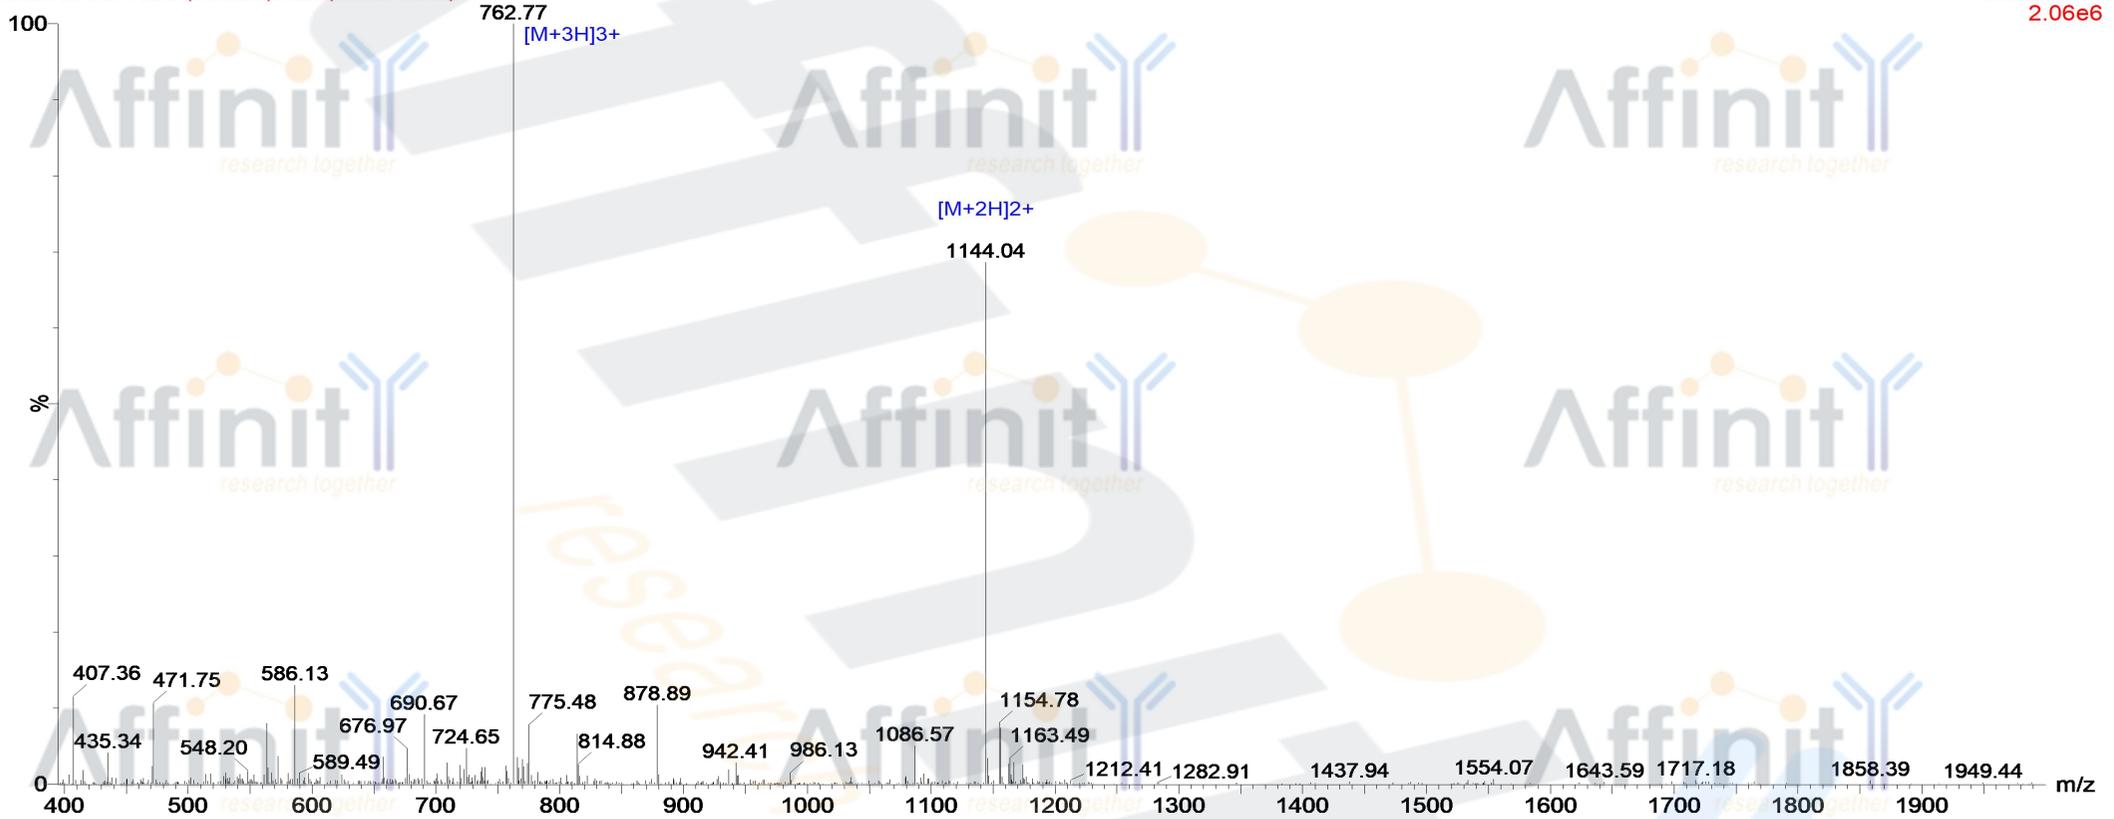

Sample Description

Analyzed date: 2014-03-10  
Analyst: YU  
Sample: I-19  
M.W.: 2284.72  
Lot. No.: P140303-CJ272380

Instrument

Waters ZQ2000  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

Probe Bias: + 4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50% H<sub>2</sub>O/50% ACN