


# MASS SPECTROMETRY REPORT

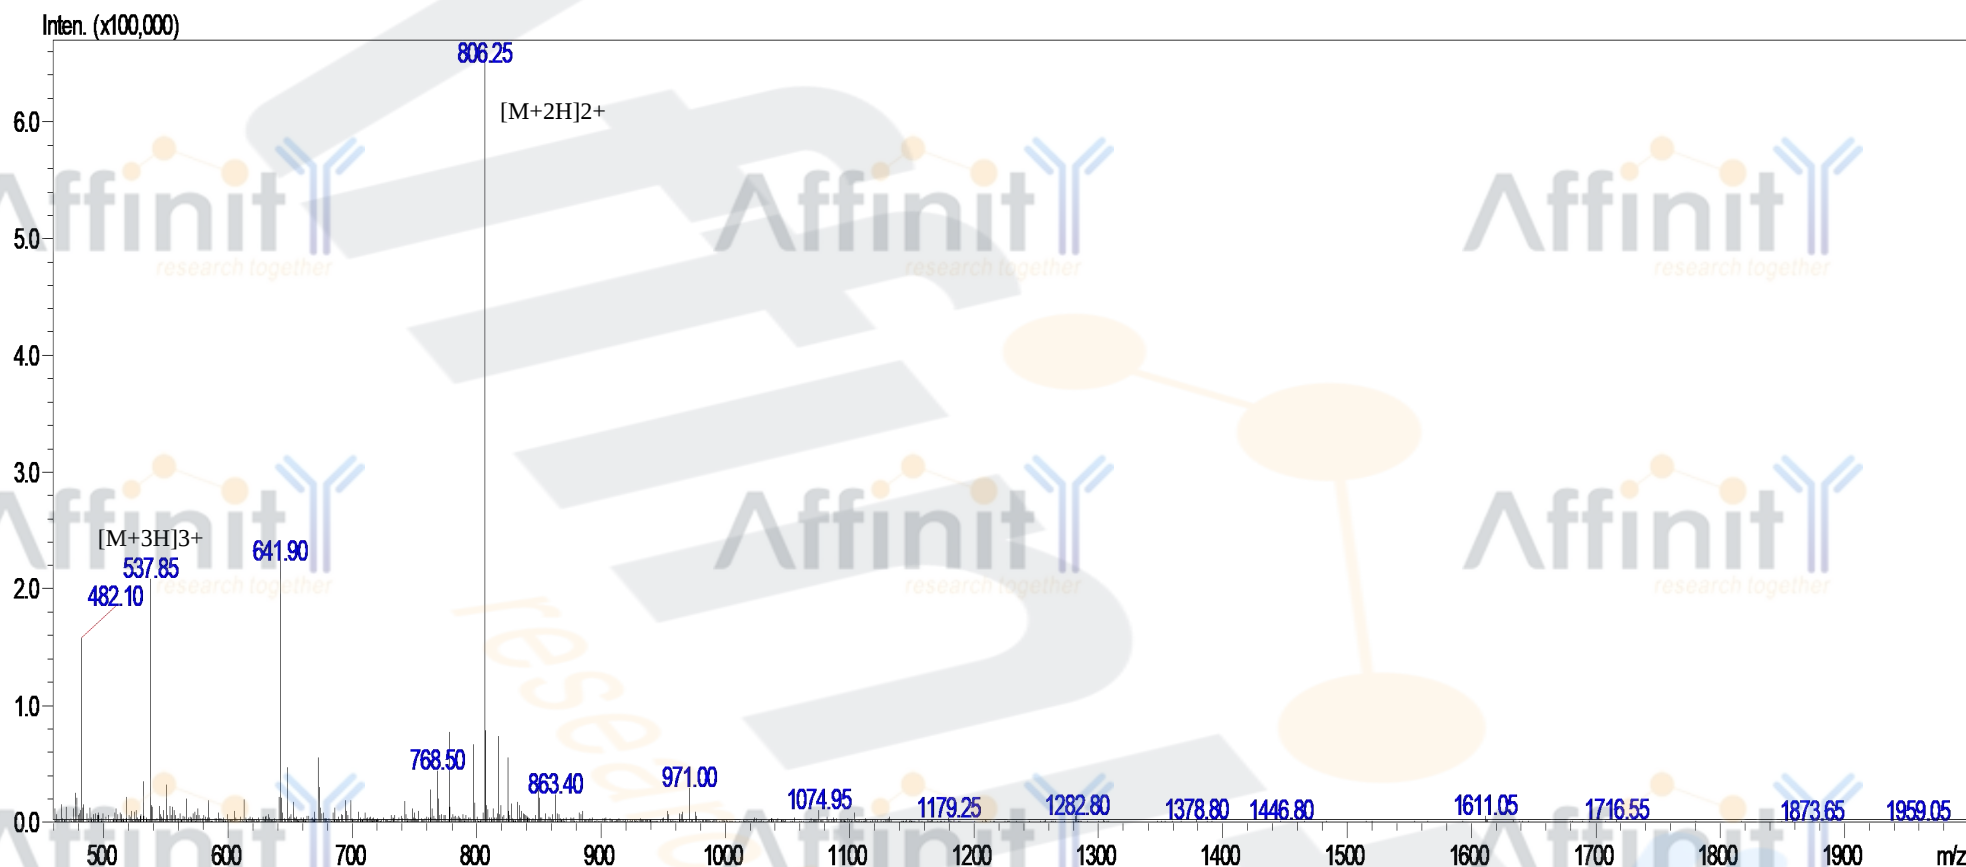

## Sample Description

Analyzed date: 2016/1/5

Analyst: Shen

Sample: A-15

M.W.: 1610.62

Lot. No.: P161219-LL627056

## Instrument

SHIMADZU LCMS-2020

## Probe:

ESI

## Probe Bias:

+ 4.5kv

## Nebulizer Gas Flow:

1.5L/min

## Detector:

1.2kv

## CDL:

-20.0v

## T. Flow:

0.2ml/min

## CDL Temp.:

250 °C

## B. Conc.:

50%H2O/50%ACN

## Block Temp.:

400 °C