


# MASS SPECTROMETRY REPORT

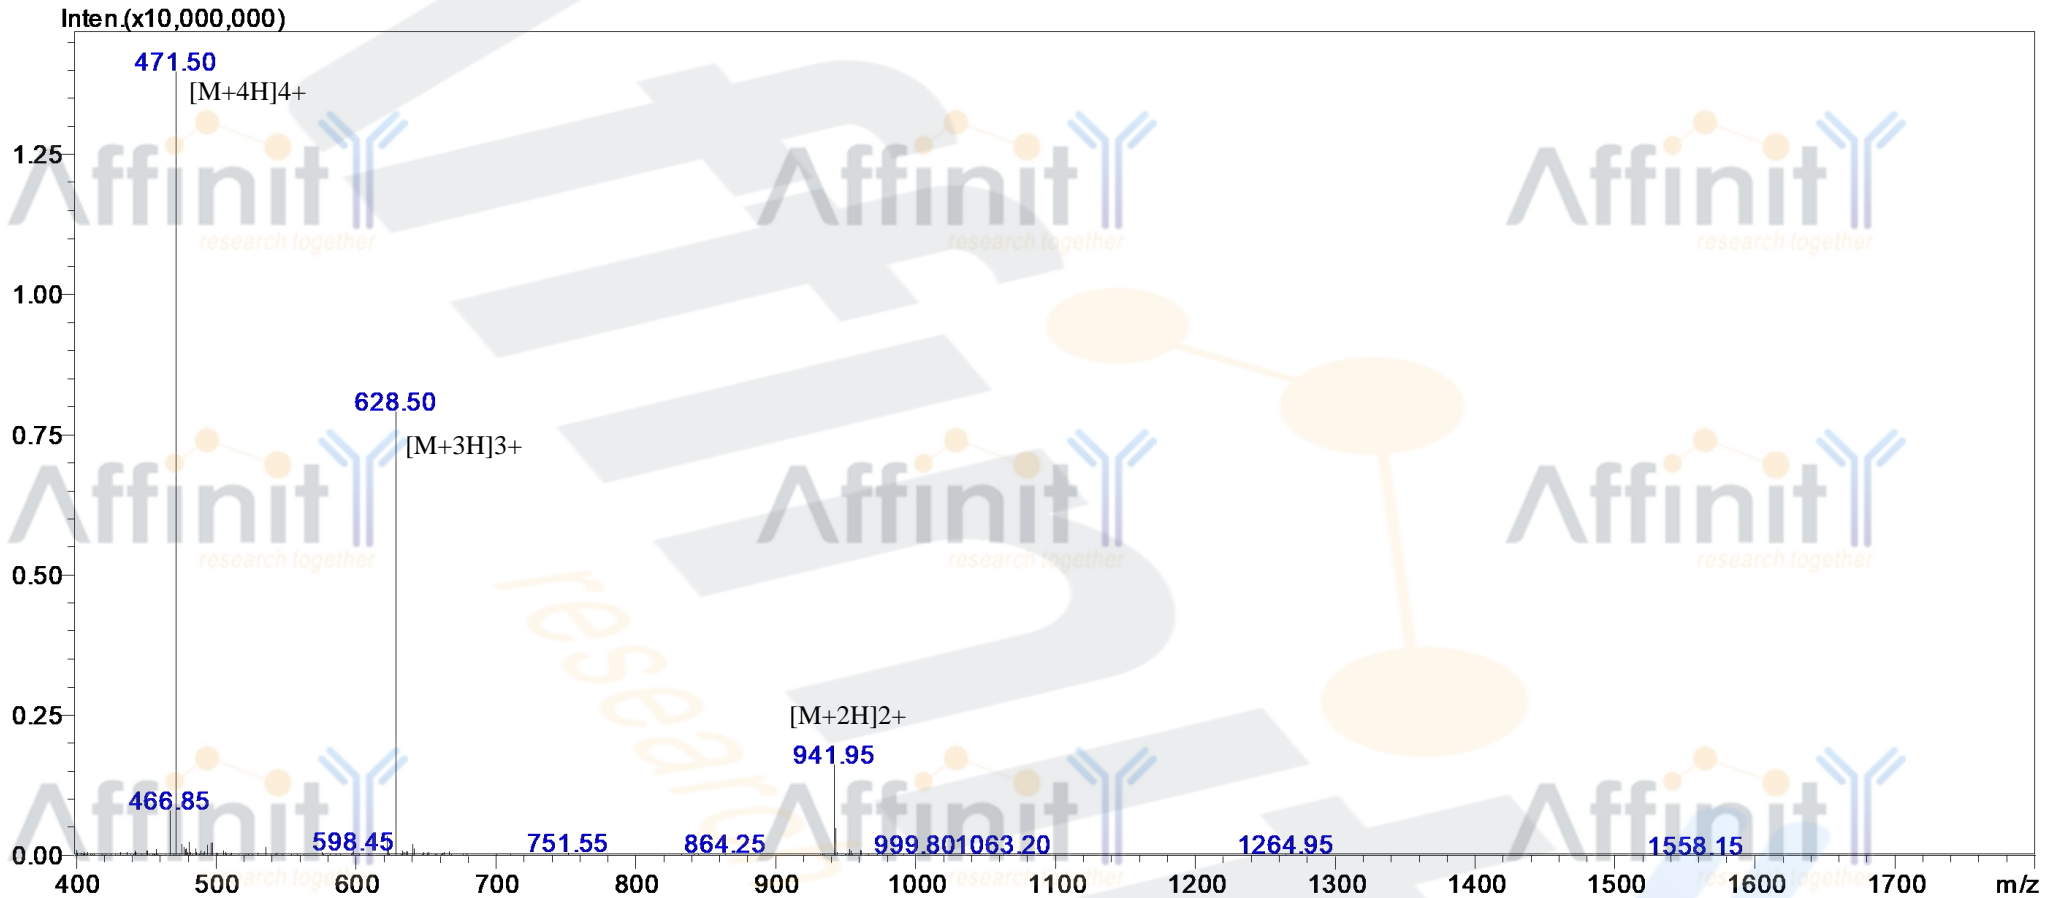

**Sample Description**

Analyzed date: 2013-7-23  
 Analyst: FENG  
 Sample: 5-404 CT-17  
 M.W.: 1882.12  
 Lot. No.: P130704-LW358316

**Instrument**

SHIMADZU LCMS-2010EV  
 Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250 °C  
 Block Temp.: 200 °C  
 Probe Bias: + 4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H2O/50% ACN