


MASS SPECTROMETRY REPORT

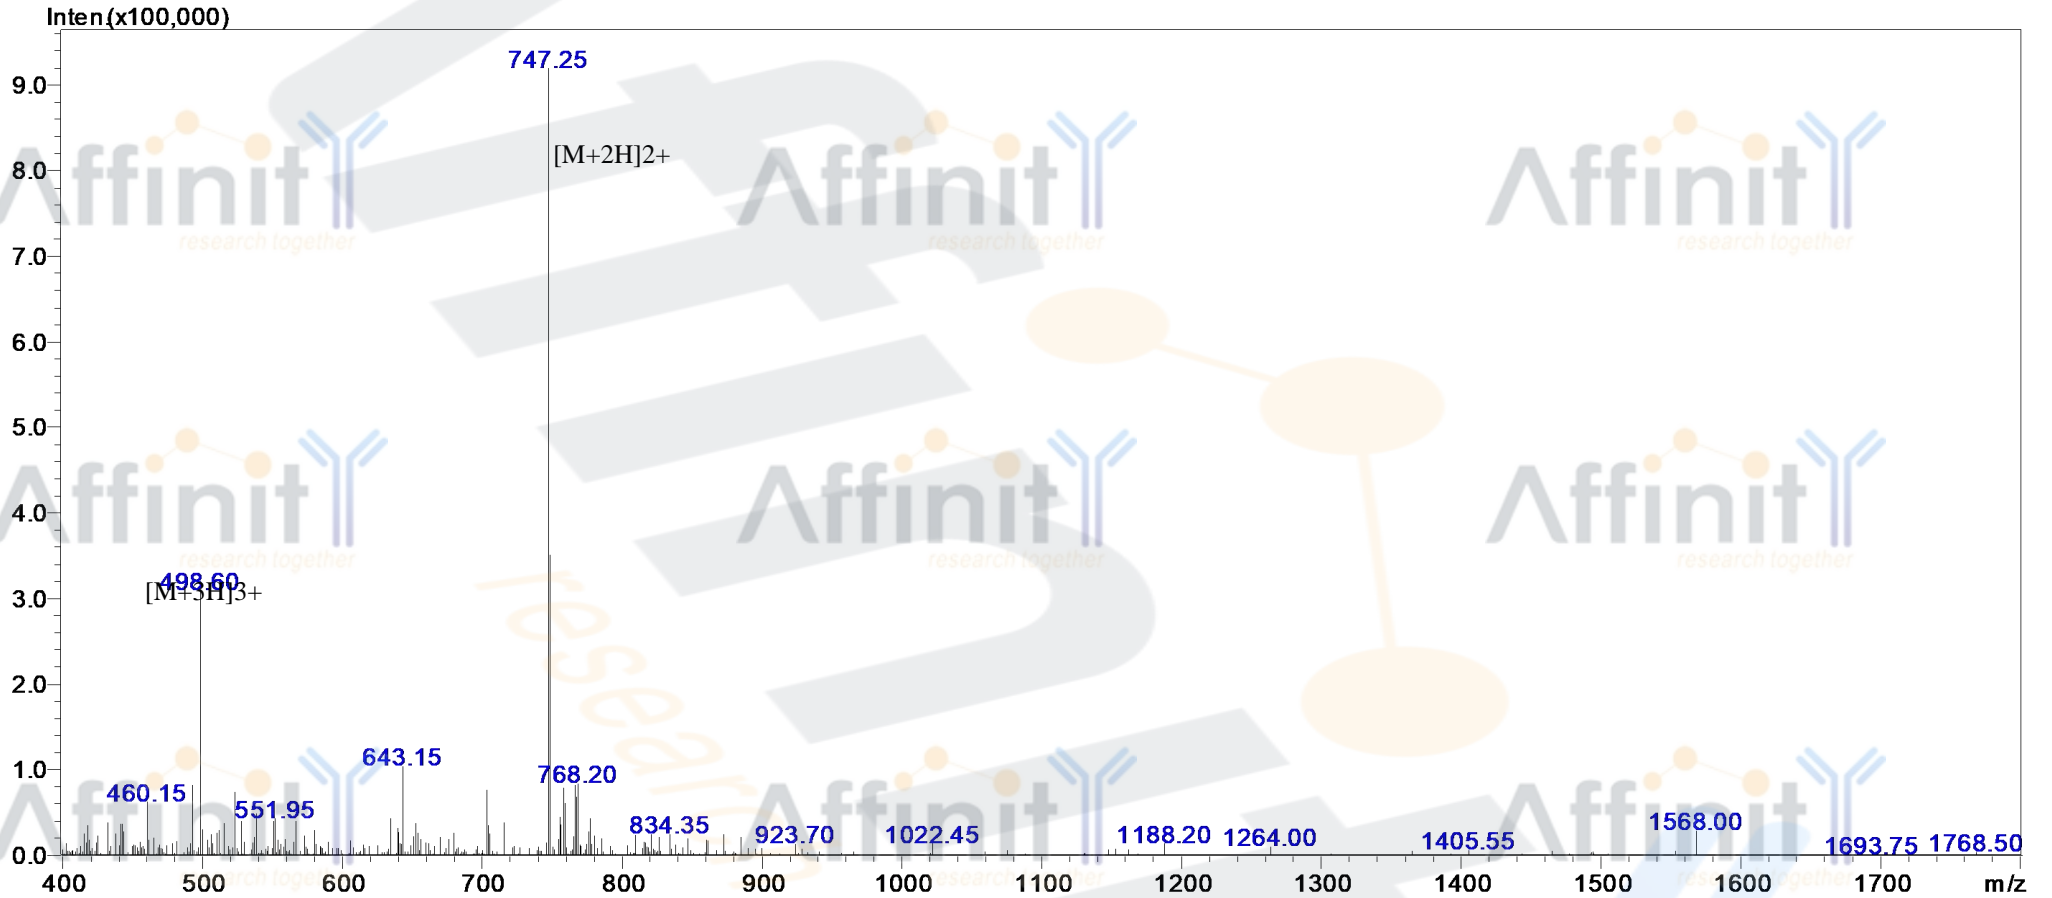

Sample Description

Analyzed date: 2013-7-30
 Analyst: FENG
 Sample: 5-420 SC-14
 M.W.: 1492.65
 Lot. No.: P130704-LW358188

Instrument

SHIMADZU LCMS-2010EV
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C
 Probe Bias: + 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H₂O/50% ACN