


MASS SPECTROMETRY REPORT

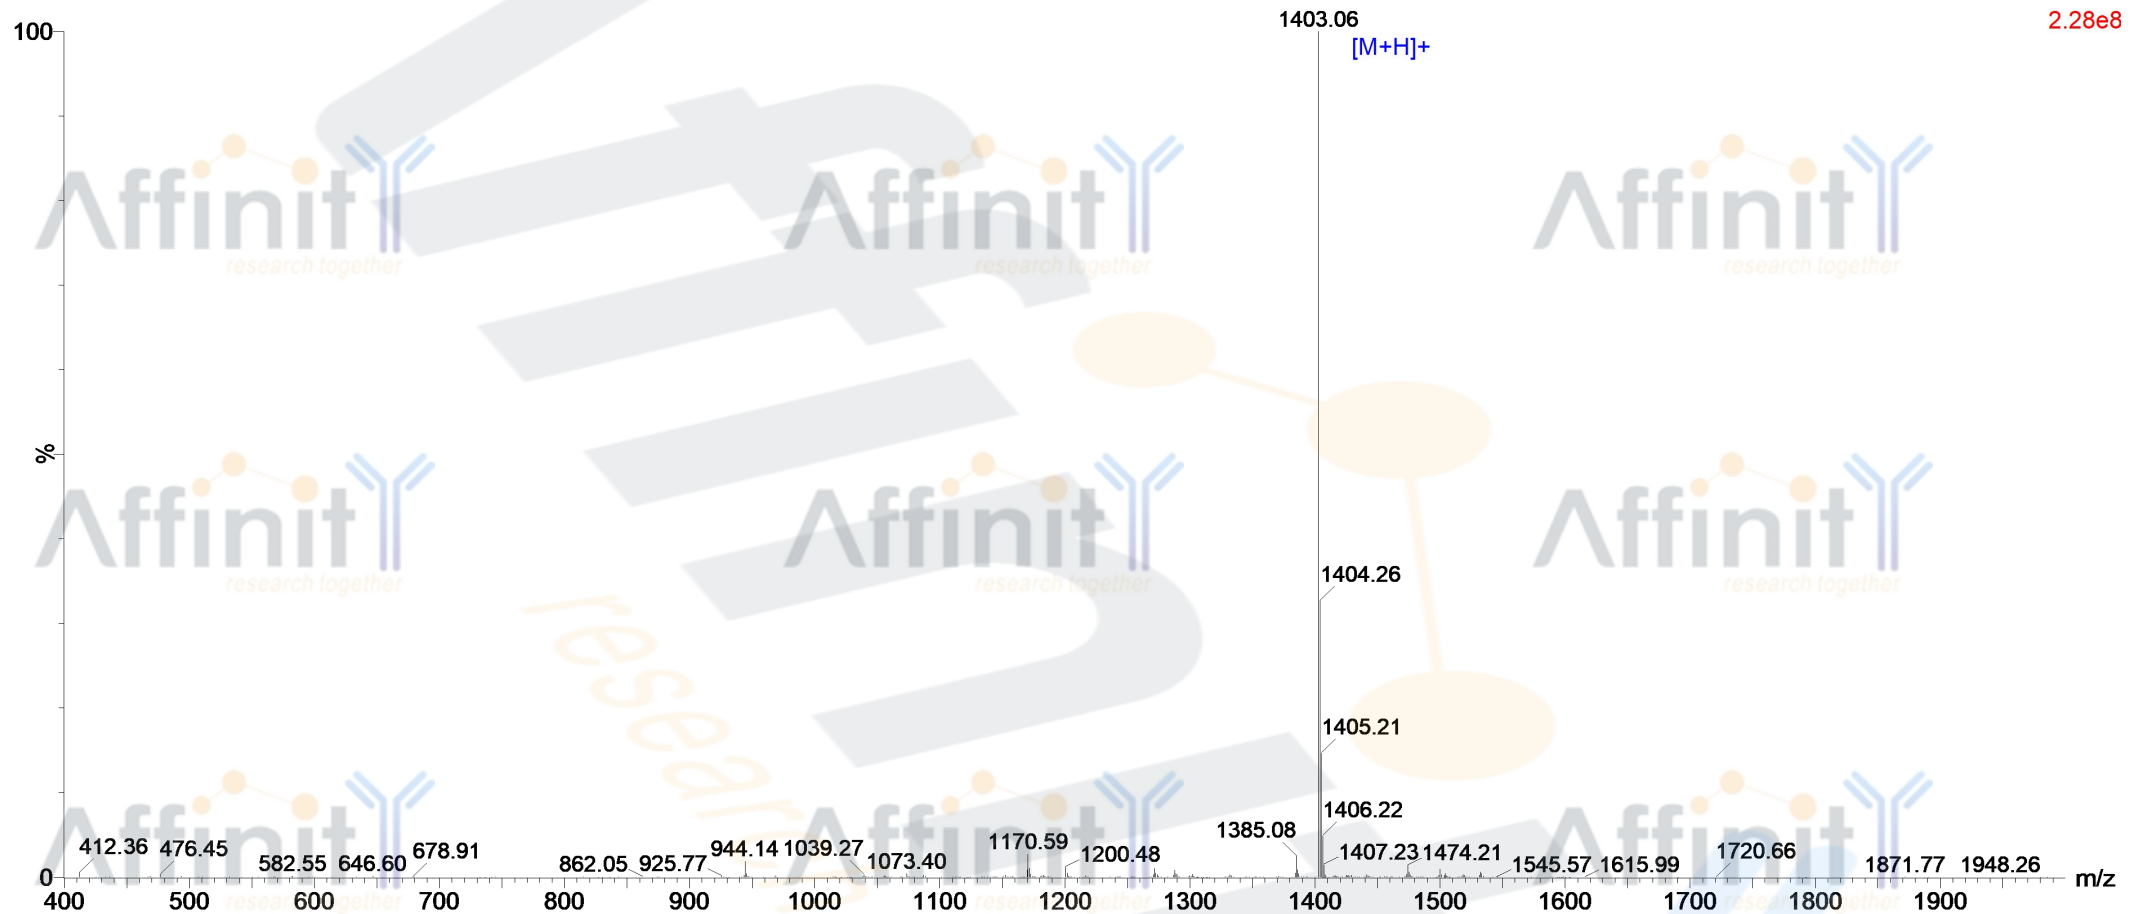

2.28e8

Sample Description

Analyzed date: 2013-07-10
Analyst: YU
Sample: 5-282 CI-13
M.W.: 1401.56
Lot. No.: P130704-ML358220

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: + 4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN