


HPLC REPORT

Sample: C-14P **Analyzed date:** 2014-10-13
Analyst: YW
Lot. No.: P140930-SY608913
Column: 4.6×250mm, Kromasil 100-5-C18
Solvent A: A: 0.1% Trifluoroacetic Acid in 100% Acetonitrile
Solvent B: B: 0.1% Trifluoroacetic Acid in 100% Water
Gradient:

	A	B
0.0min	18%	82%
25.0min	43%	57%
25.1min	100%	0%
30.0min	Stop	

Volume: 5µl
Wavelength: 220nm
Flow rate: 1.0ml/min

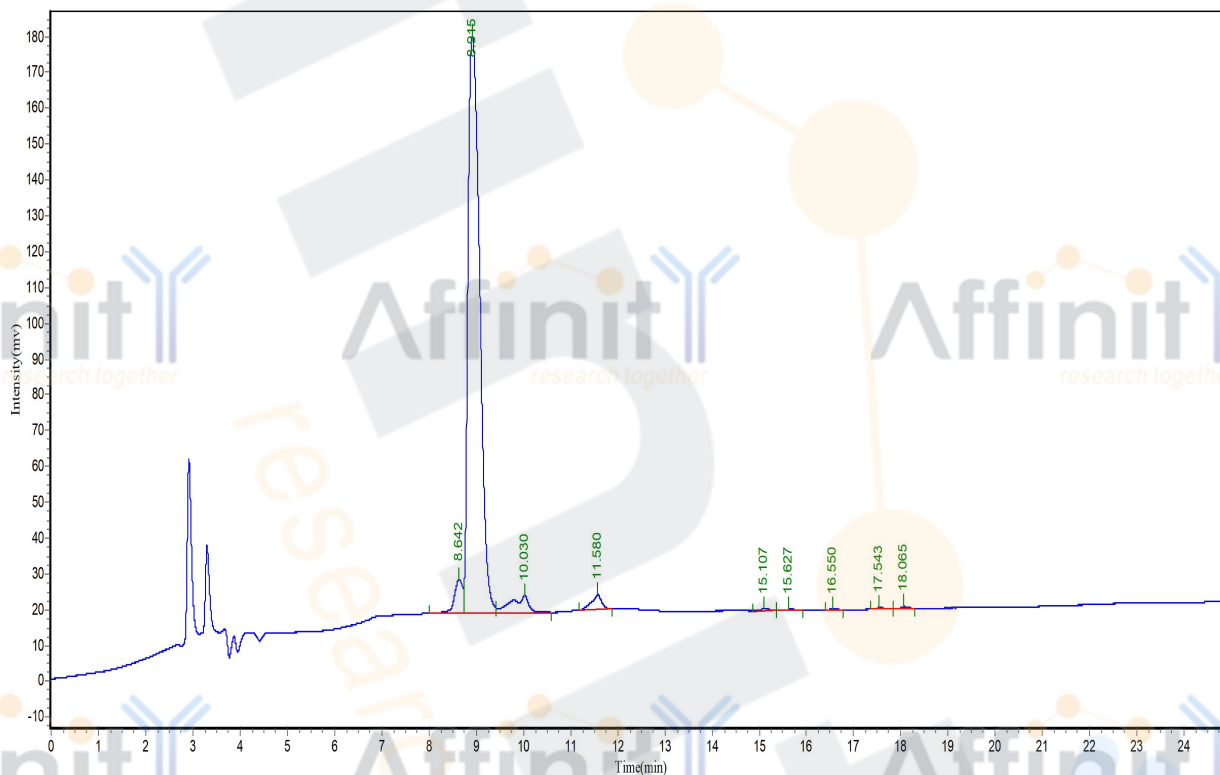

Peak	Time	Height	Area	Conc.
1	8.642	9441.195	115341.938	3.7562
2	8.915	161157.953	2750728.500	89.5798
3	10.030	4599.312	122796.555	3.9990
4	11.580	4108.549	59615.984	1.9414
5	15.107	573.892	6494.076	0.2115
6	15.627	239.256	3945.502	0.1285
7	16.550	364.205	2718.393	0.0885
8	17.543	361.297	4408.374	0.1436
9	18.065	551.490	4651.948	0.1515

Total 100.000