


# MASS SPECTROMETRY REPORT

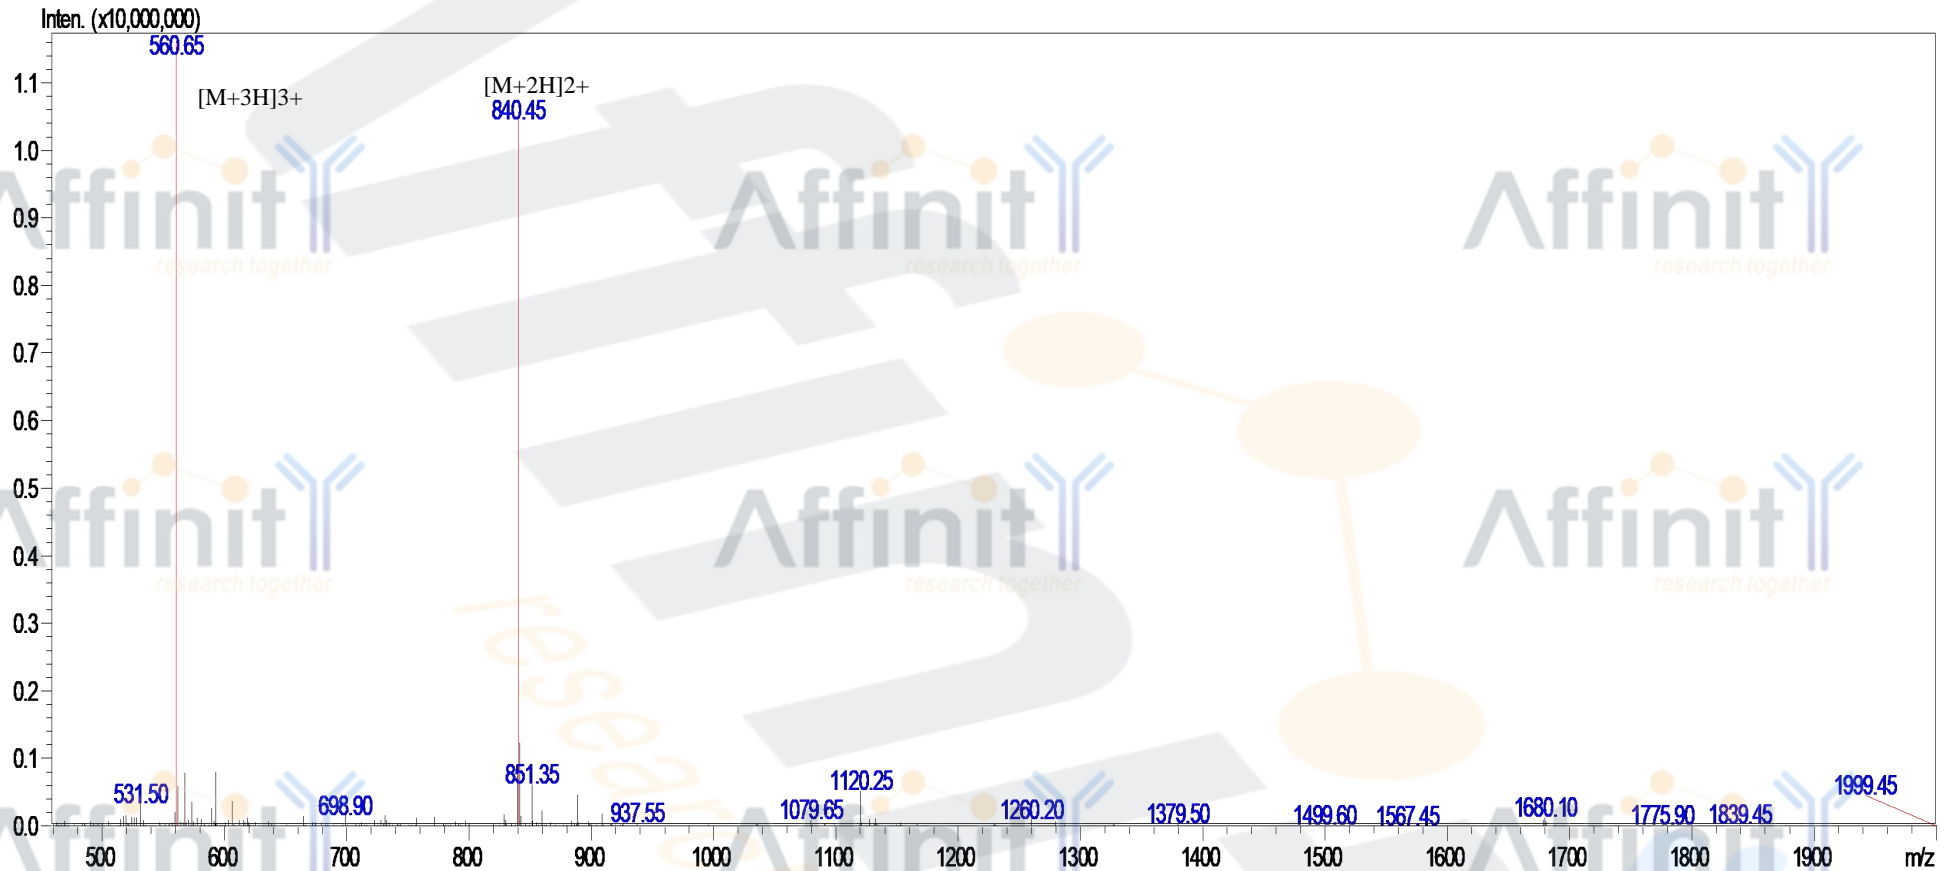

Sample Description  
 Analyzed date: 2014/10/10  
 Analyst: Shen  
 Sample: C-14  
 M.W.: 1678.94  
 Lot. No.: P140922-LL609288

Instrument SHIMADZU LCMS-2020  
 Probe: ESI Probe Bias: + 4.5kv  
 Nebulizer Gas Flow: 1.5L/min Detector: 1.2kv  
 CDL: -20.0v T. Flow: 0.2ml/min  
 CDL Temp.: 250 °C B. Conc.: 50% H2O/50% ACN  
 Block Temp.: 400 °C