

MASS SPECTROMETRY REPORT


29-Sep-2017
10:50:52

Probe: ESI
Cone: 50v
Desovation Temp :350

Capillary:3.00KV
Extractor: 5v
Gas Flow : 350

Scan ES-
4.49e4

170929-23- 34 (0.628) Cm (33:37)

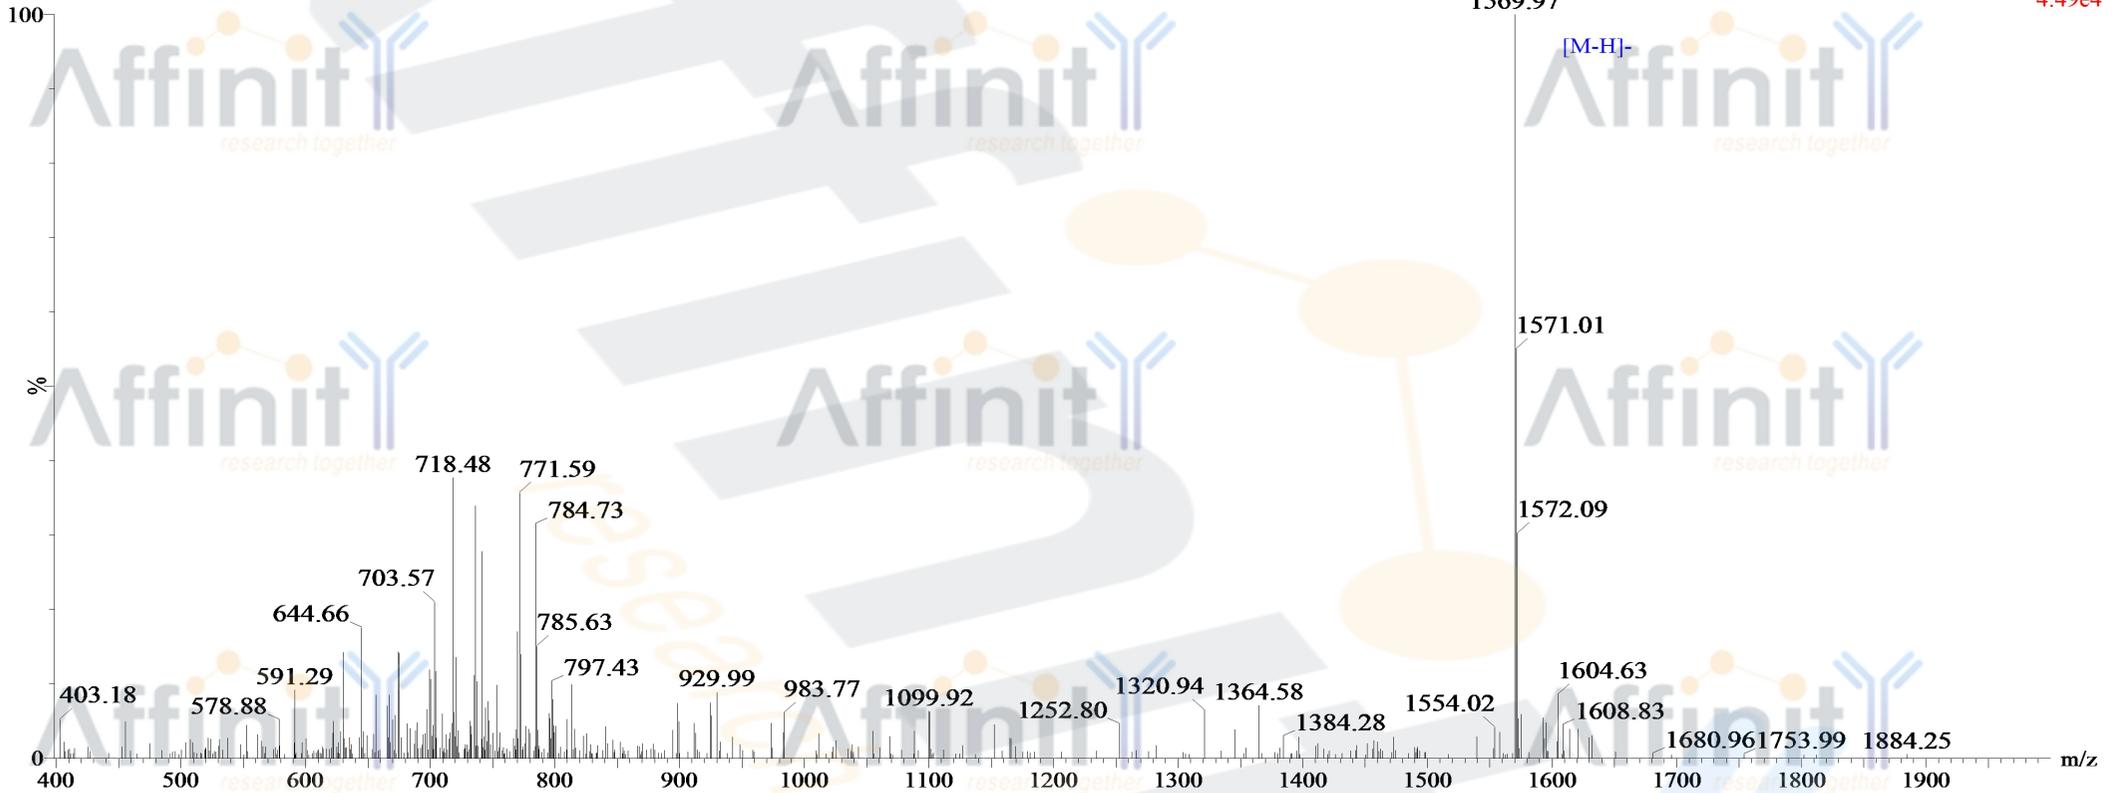

Sample Description

Analyzed date: 2014-09-29
 Analyst: YU
 Sample: C-13P
 M.W.: 1571.65
 Lot. No.: P140921-CJ609732

Instrument

Waters ZQ2000
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C

Probe Bias: + 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H2O/50% ACN