


MASS SPECTROMETRY REPORT

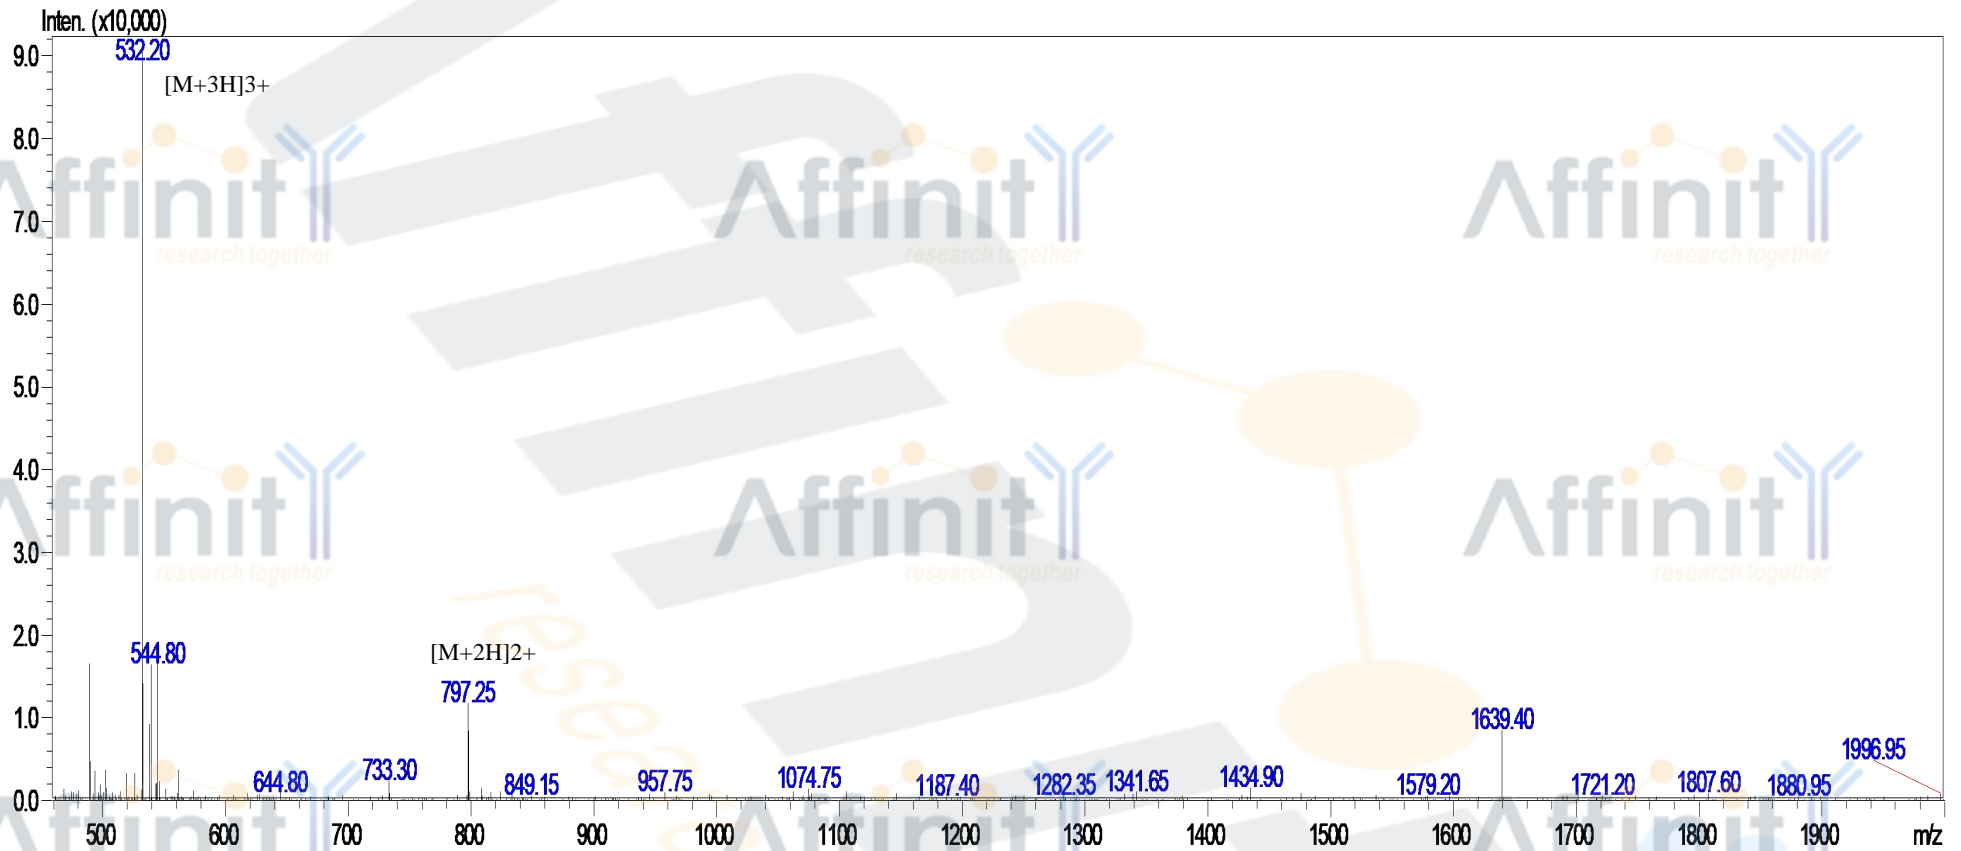

Sample Description
 Analyzed date: 2014/9/28
 Analyst: Shen
 Sample: C-13
 M.W.: 1592.69
 Lot. No.: P140925-YS609436

Instrument: SHIMADZU LCMS-2020
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 400 °C
 Probe Bias: + 4.5kv
 Detector: 1.2kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H₂O/50% ACN