


MASS SPECTROMETRY REPORT

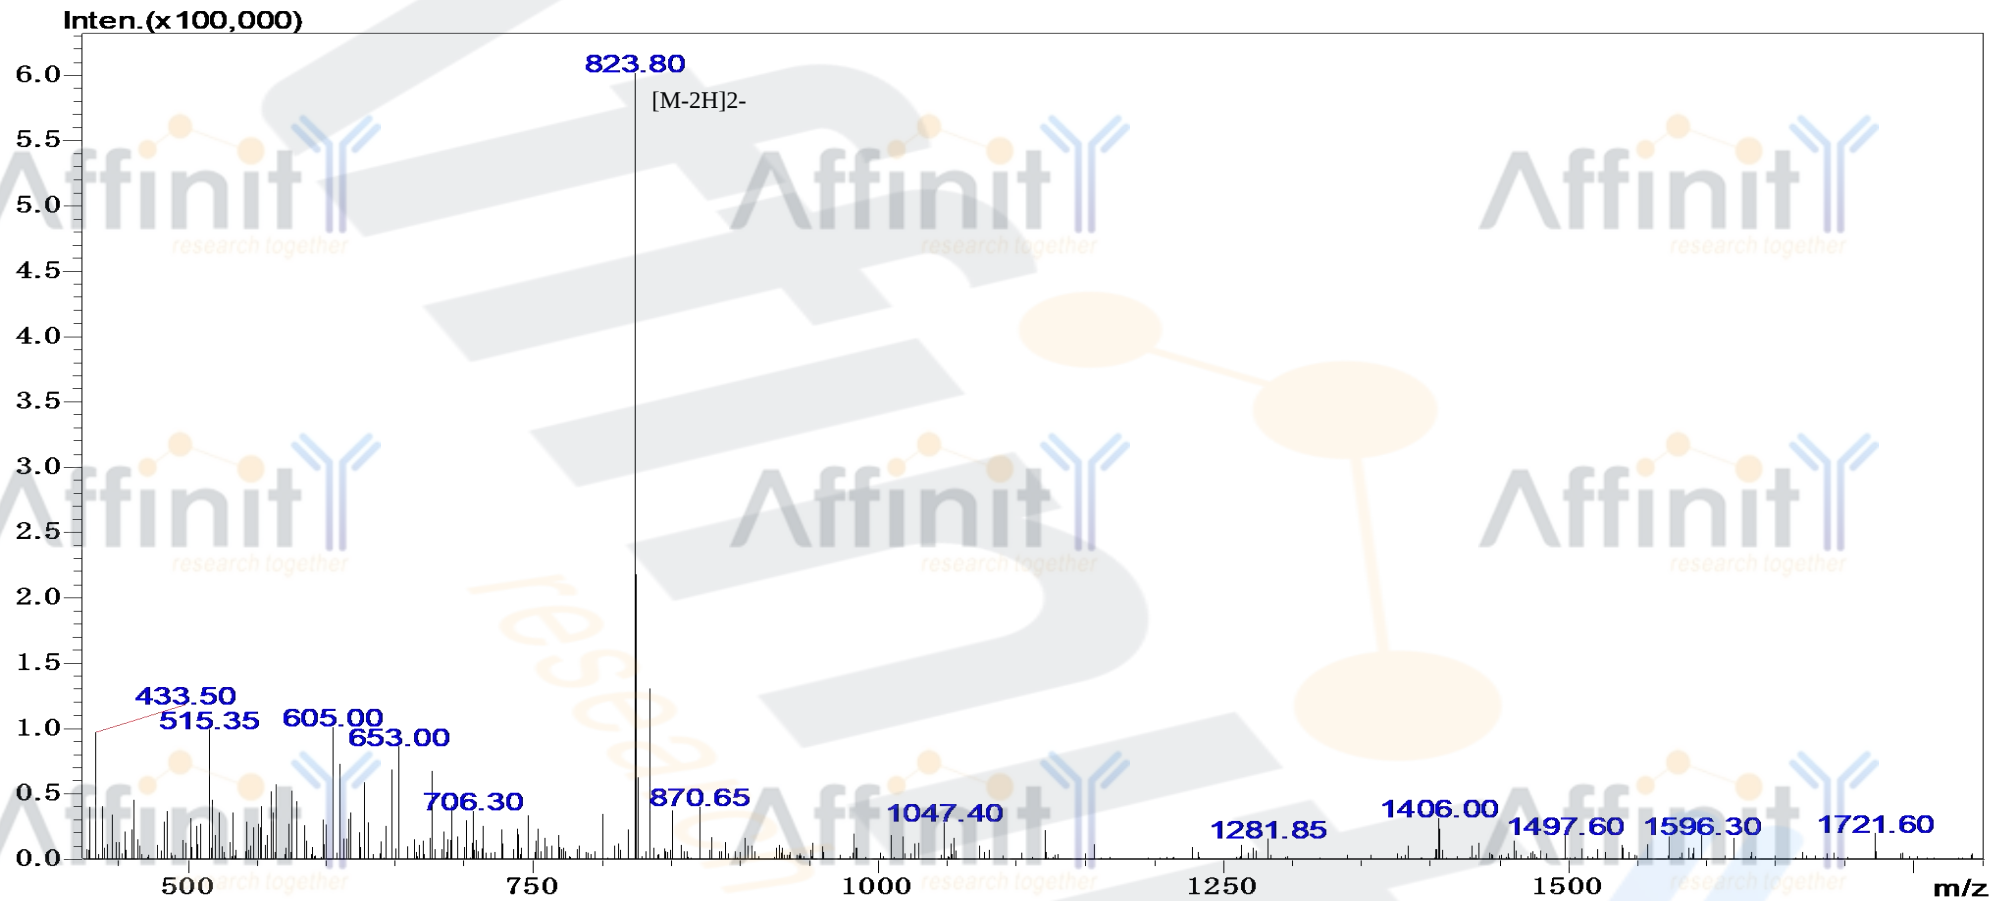

Sample Description

Analyzed date: 2014-10-14
Analyst: Xu
Sample: C-13P
M.W.: 1649.73
Lot. No.: P140922--YJ608758

Instrument

SHIMADZU LCMS-2010EV
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C
Probe Bias: + 4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H₂O/50%ACN