


# MASS SPECTROMETRY REPORT

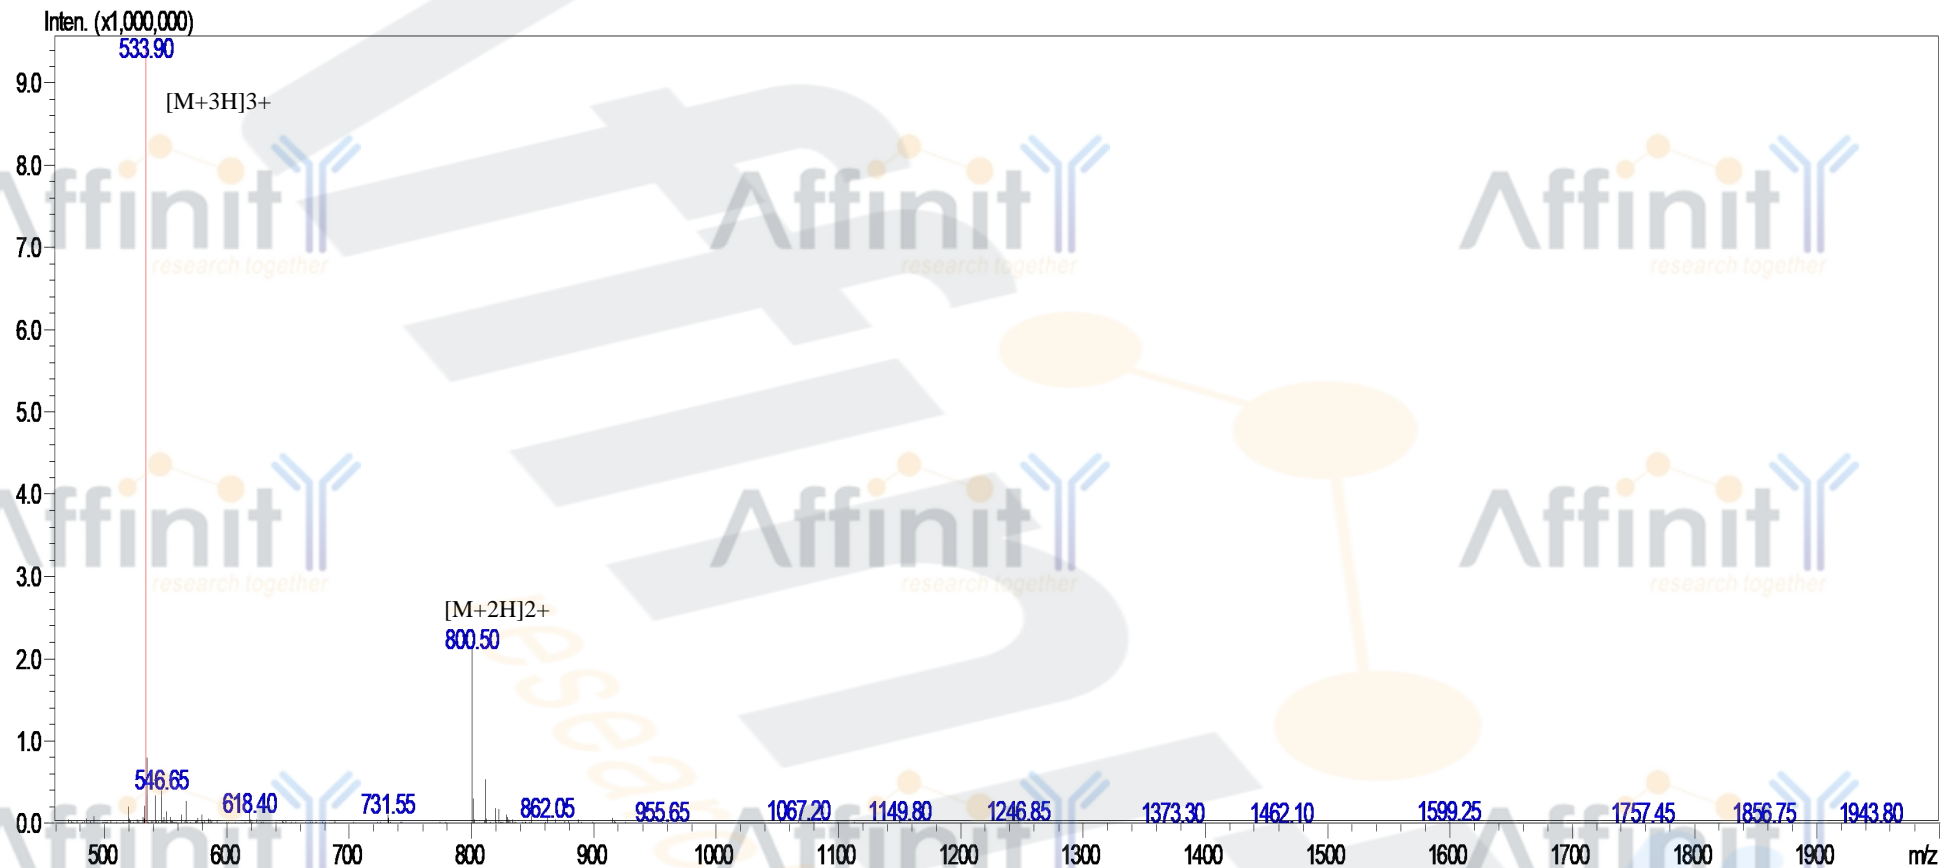

Sample Description  
 Analyzed date: 2014/10/9  
 Analyst: Shen  
 Sample: C-14  
 M.W.: 1598.94  
 Lot. No.: P140922-LL608482

Instrument: SHIMADZU LCMS-2020  
 Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250 °C  
 Block Temp.: 400 °C  
 Probe Bias: + 4.5kv  
 Detector: 1.2kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H<sub>2</sub>O/50% ACN