


MASS SPECTROMETRY REPORT

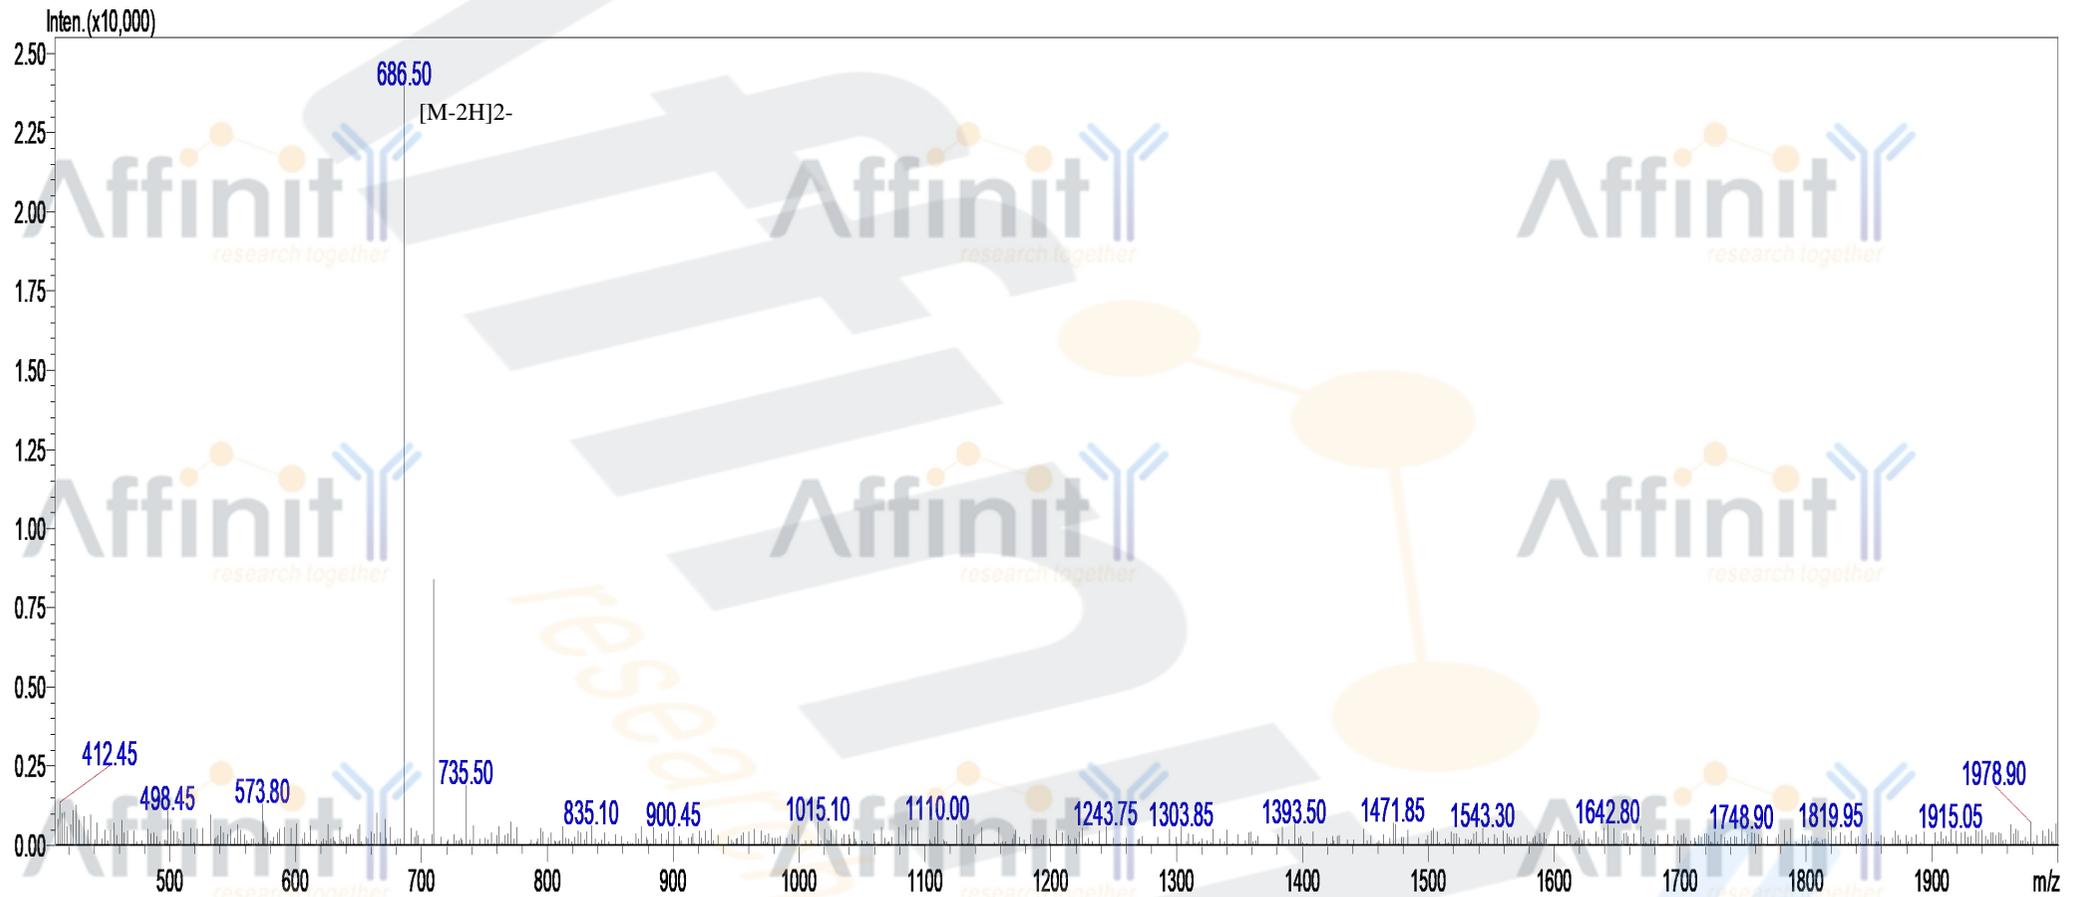

Sample Description

Analyzed date: 2014-9-29
 Analyst: SHAO
 Sample: C-13
 M.W.: 1375.67
 Lot. No.: P140921-HS608550

Instrument

SHIMADZU LCMS-2020
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250°C
 Block Temp.: 200°C
 Probe Bias: + 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H₂O/50% ACN