


MASS SPECTROMETRY REPORT

Inten. (x 100,000)

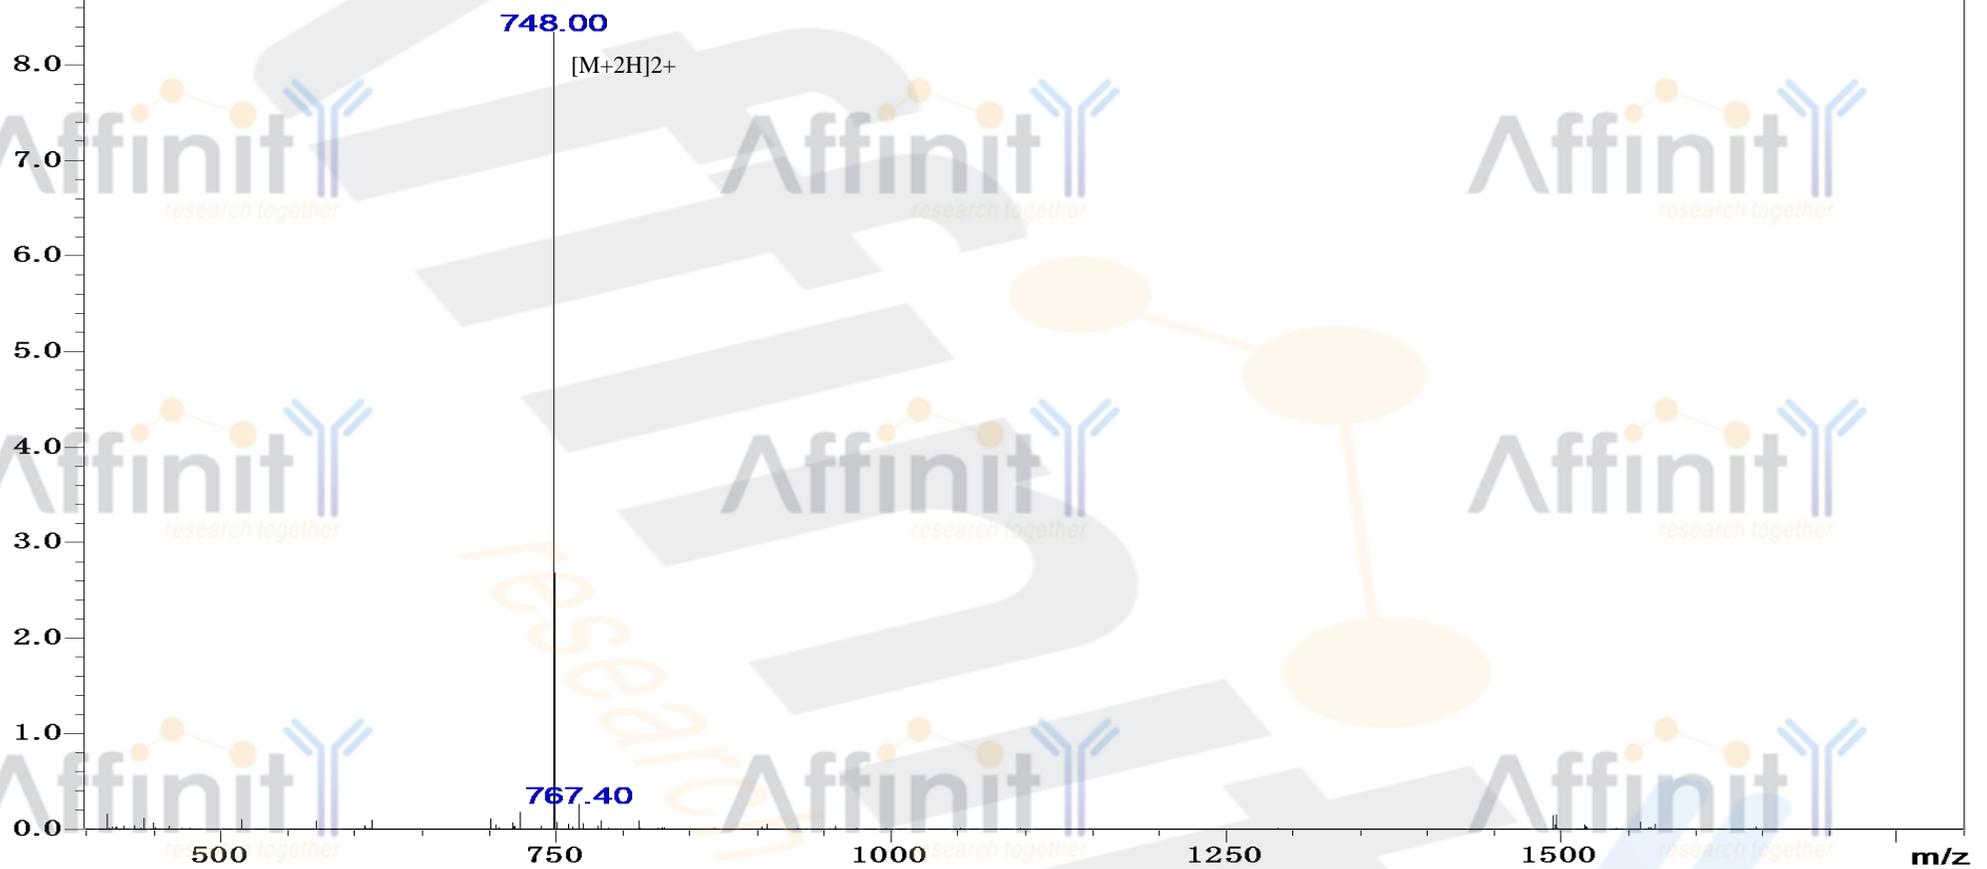

Sample Description

Analyzed date: 2014-9-28  
 Analyst: Xu  
 Sample: A-12  
 M.W.: 1494.67  
 Lot. No.: P140922-YS608596

Instrument

Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250 °C  
 Block Temp.: 200 °C

SHIMADZU LCMS-2010EV

Probe Bias: + 4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H2O/50% ACN