


# MASS SPECTROMETRY REPORT

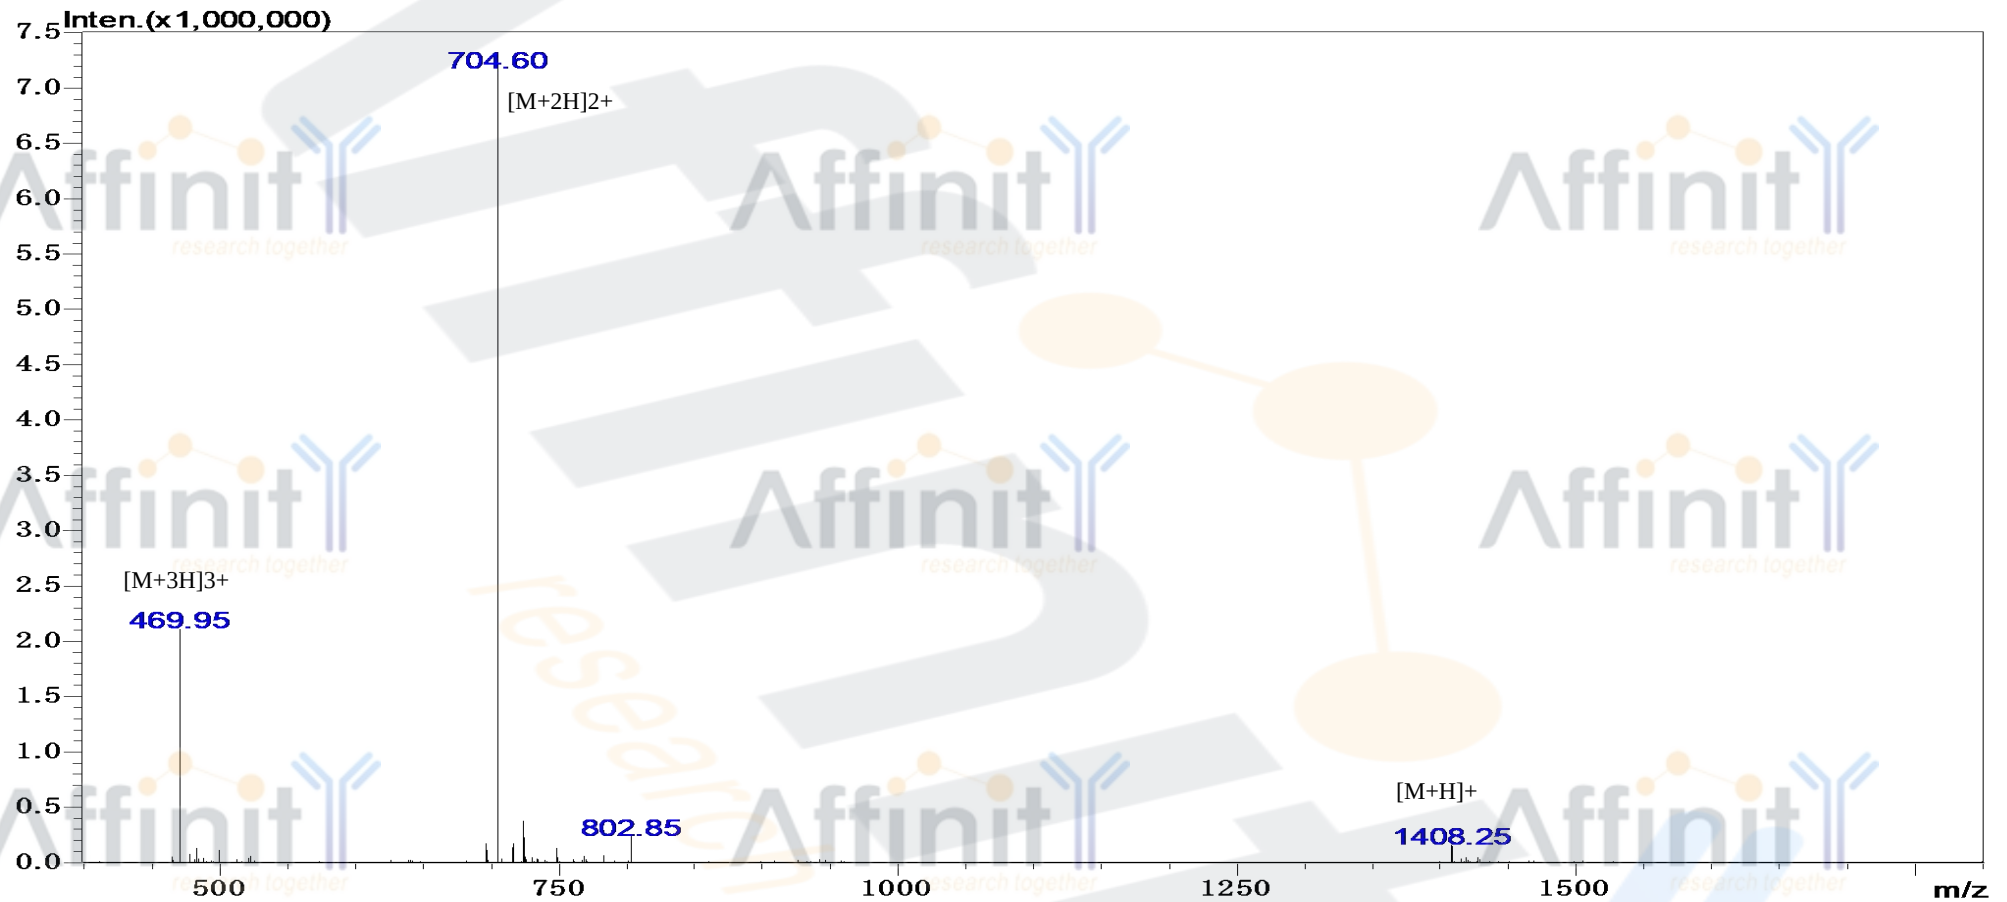

## Sample Description

Analyzed date: 2014-9-27  
Analyst: Xu  
Sample: C-12  
M.W.: 1407.51  
Lot. No.: P140922-YJ608753

## Instrument

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

## SHIMADZU LCMS-2010EV

Probe Bias: + 4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50%H2O/50%ACN