


MASS SPECTROMETRY REPORT

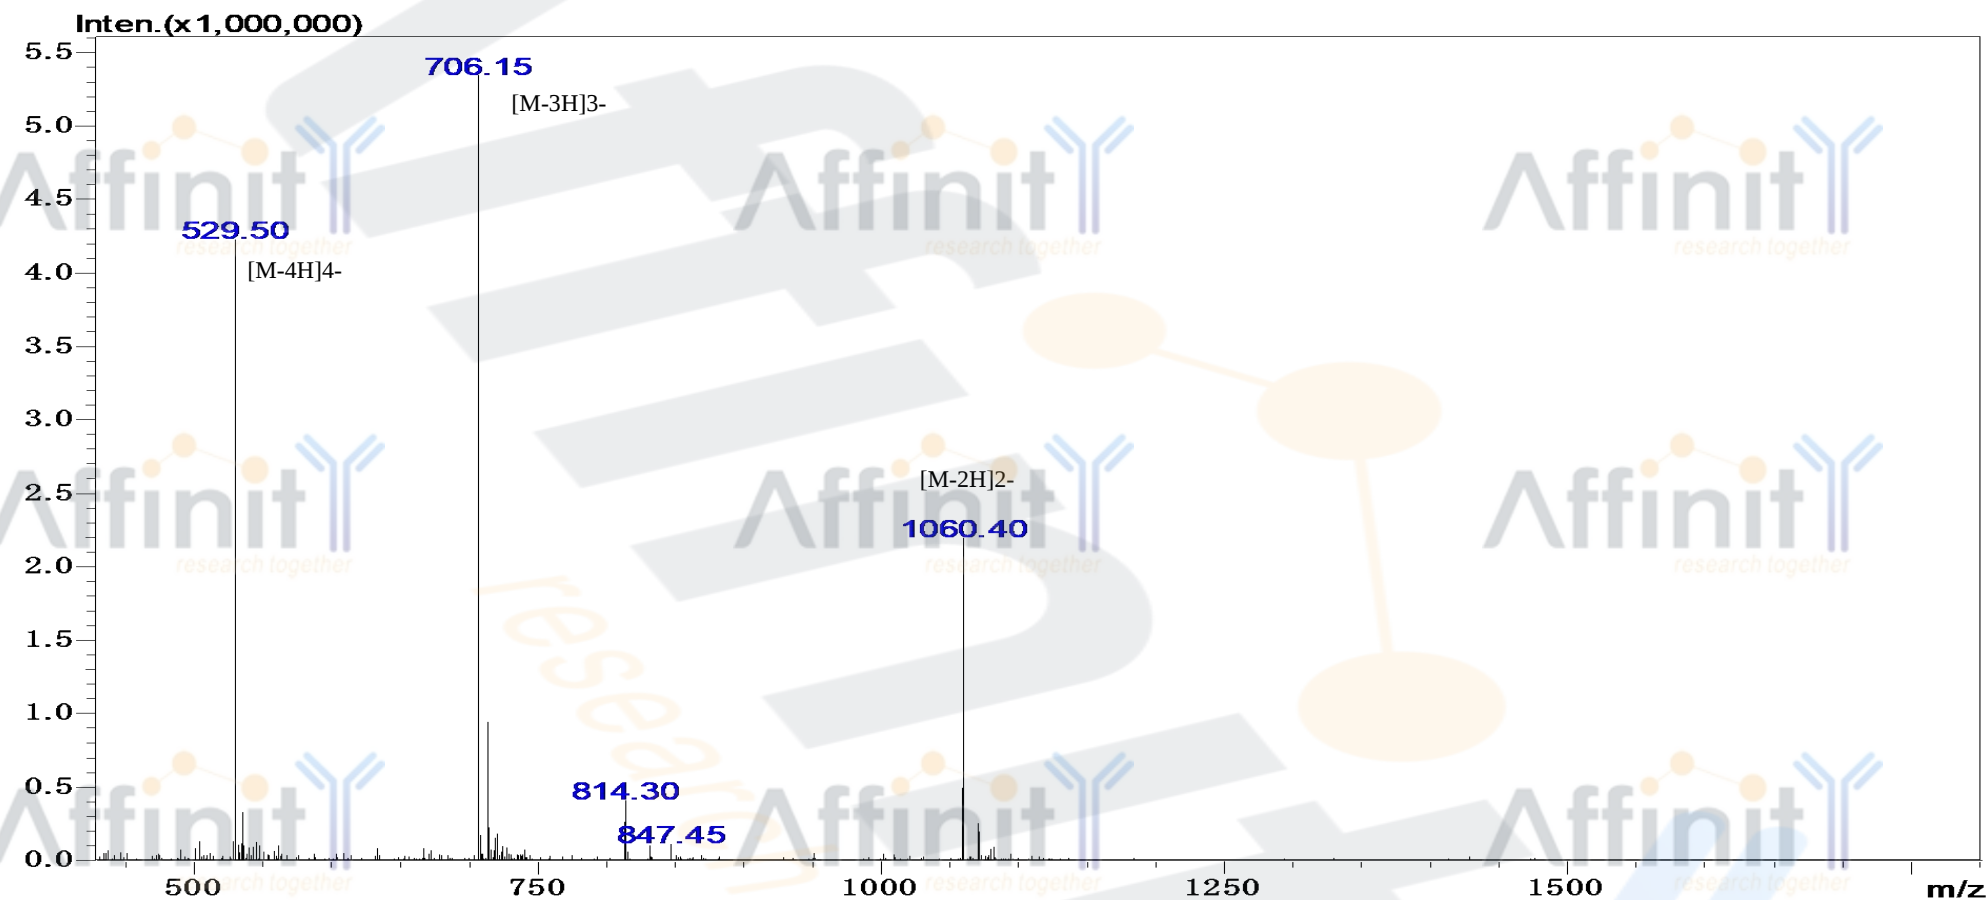

Sample Description

Analyzed date: 2014-7-15
 Analyst: Xu
 Sample: Y-16
 M.W.: 2122.10
 Lot. No.: P140705-YJ328673

Instrument

SHIMADZU LCMS-2010EV
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C
 Probe Bias: + 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50%H2O/50%ACN