


MASS SPECTROMETRY REPORT

09-Jun-2017
16:47:12

Probe: ESI
Cone: 50v
Desolvation Temp :350
Capillary:3.00KV
Extractor: 5v
Gas Flow : 350
Scan ES-
1.71e4

170609-38- 29 (0.536) Cm (24:29)

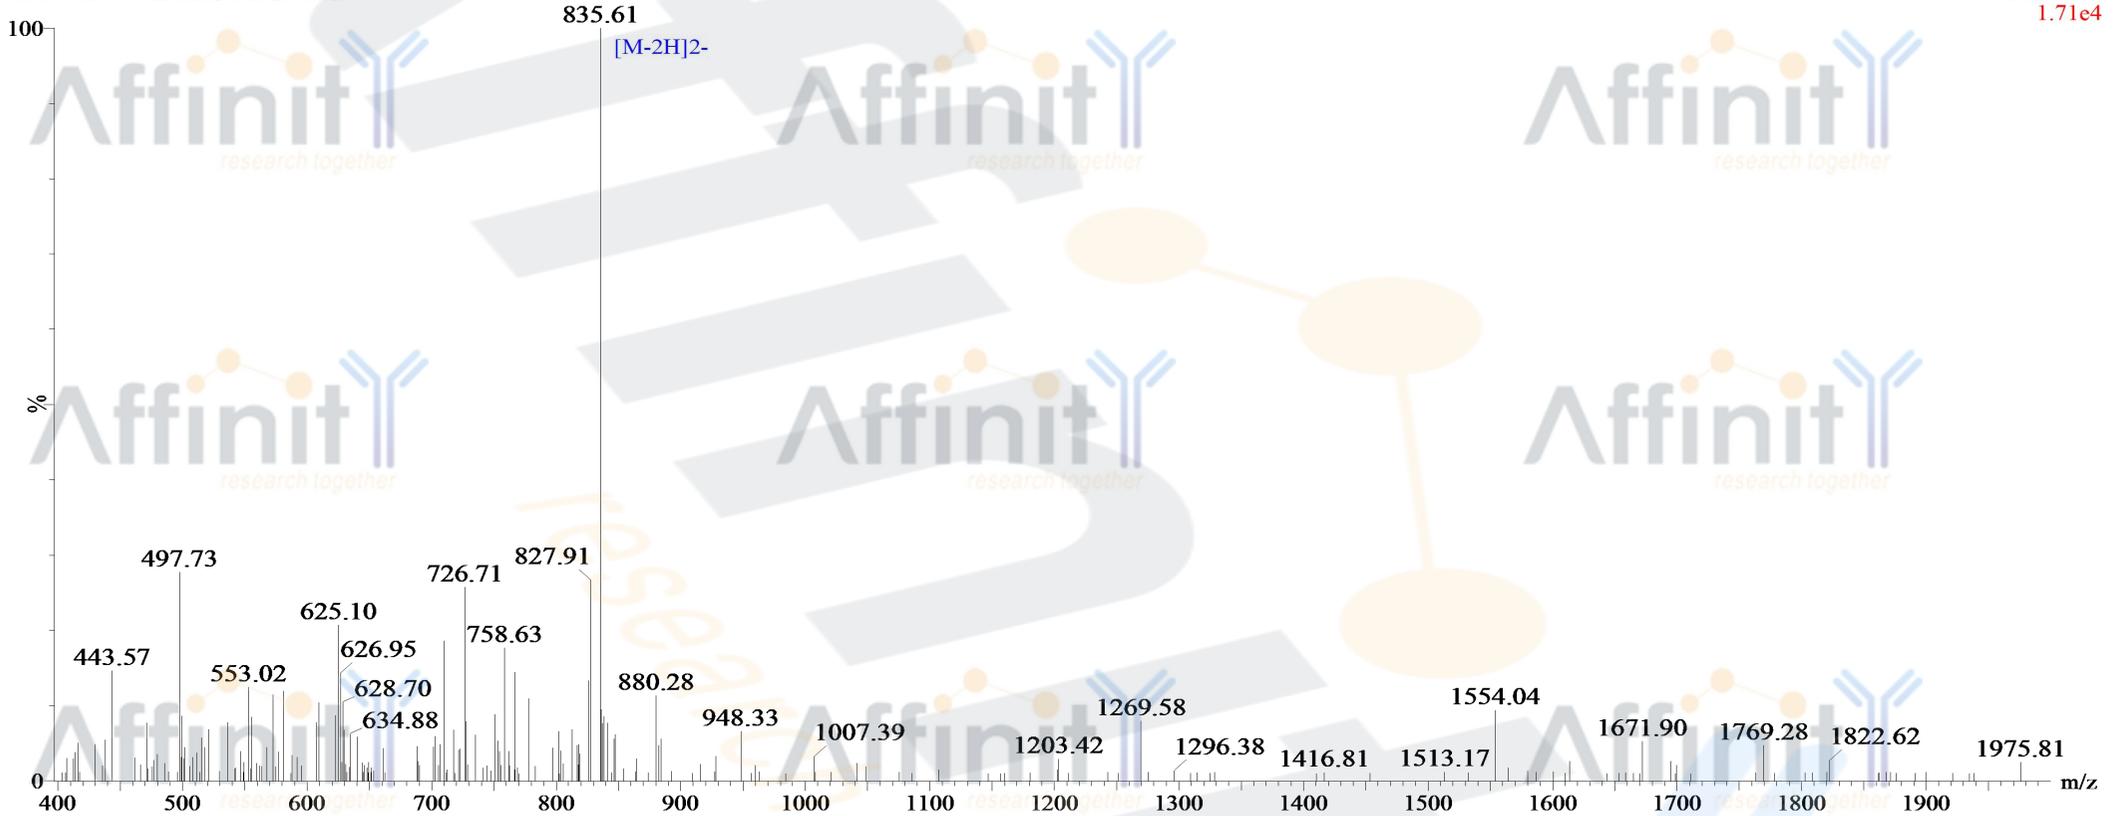

Sample Description

Analyzed date: 2014-06-09
Analyst: YU
Sample: E-14p
M.W.: 1672.73
Lot. No.: P140602-CJ546398

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: + 4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50% ACN