


MASS SPECTROMETRY REPORT

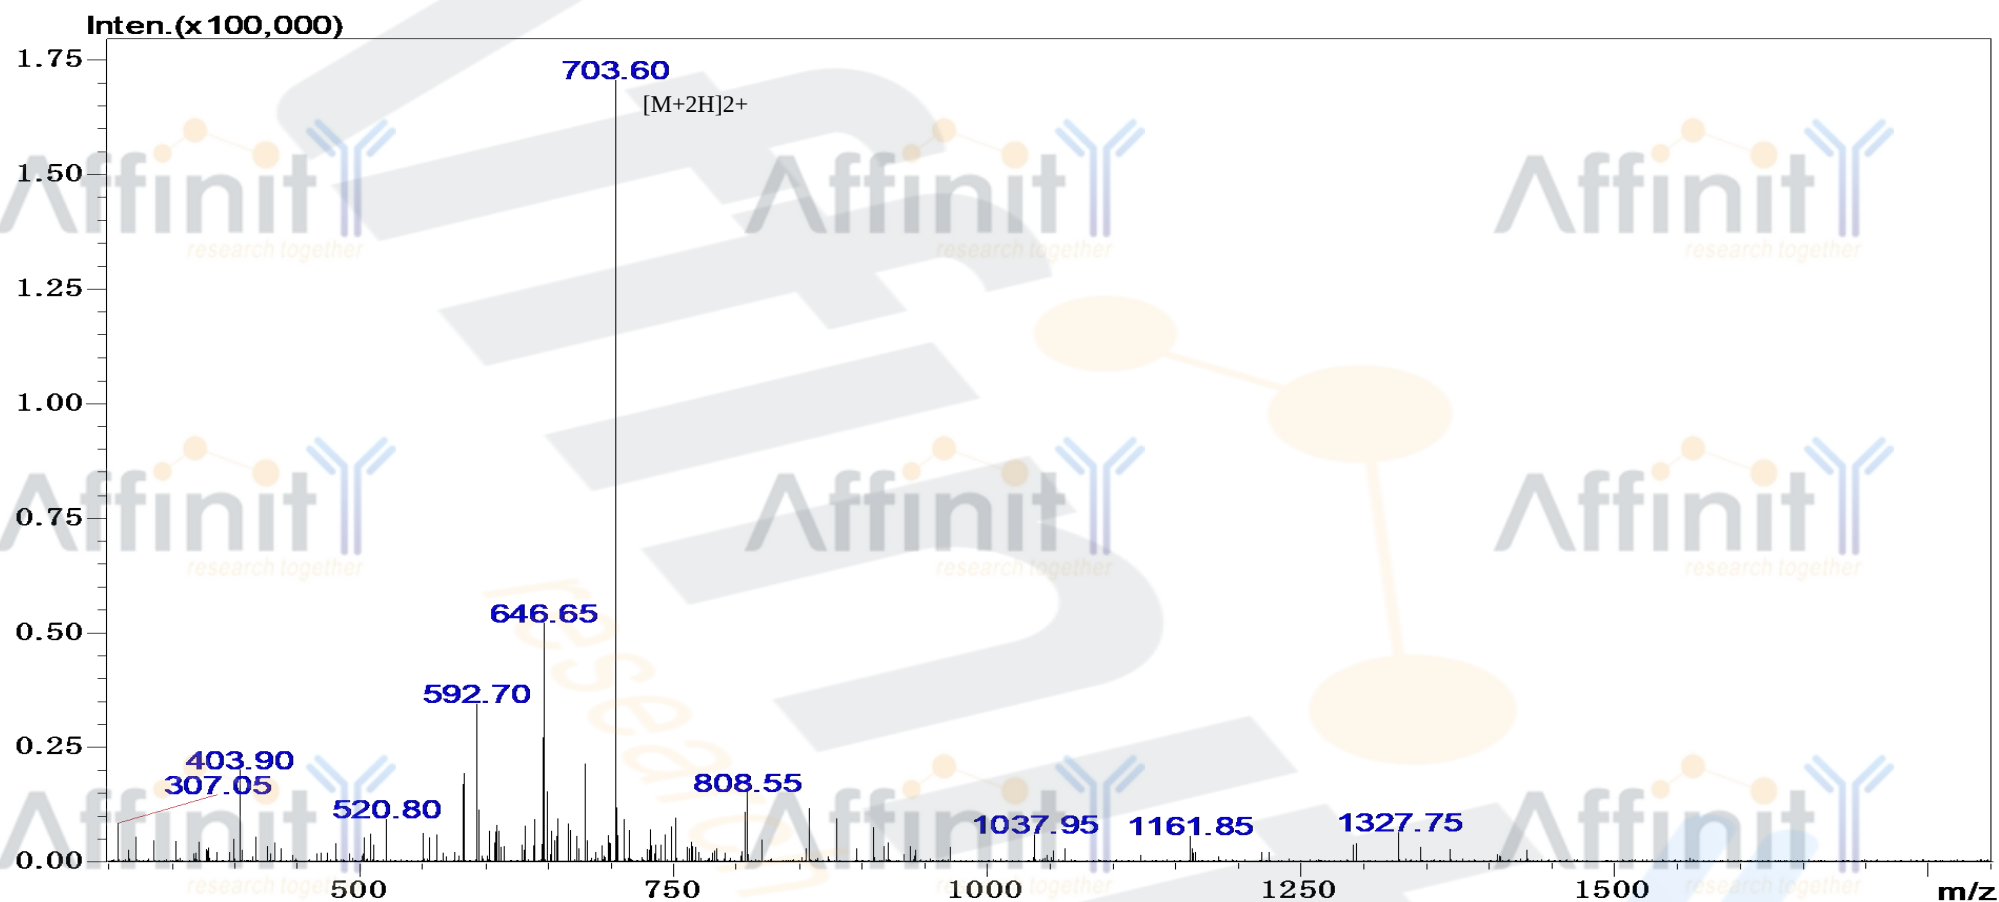

Sample Description

Analyzed date: 2014-7-18
 Analyst: Xu
 Sample: C-12(P)-2
 M.W.: 1405.49
 Lot. No.: P140710-MX594699

Instrument

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C

SHIMADZU LCMS-2010EV

Probe Bias: + 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50%H2O/50%ACN