


# MASS SPECTROMETRY REPORT

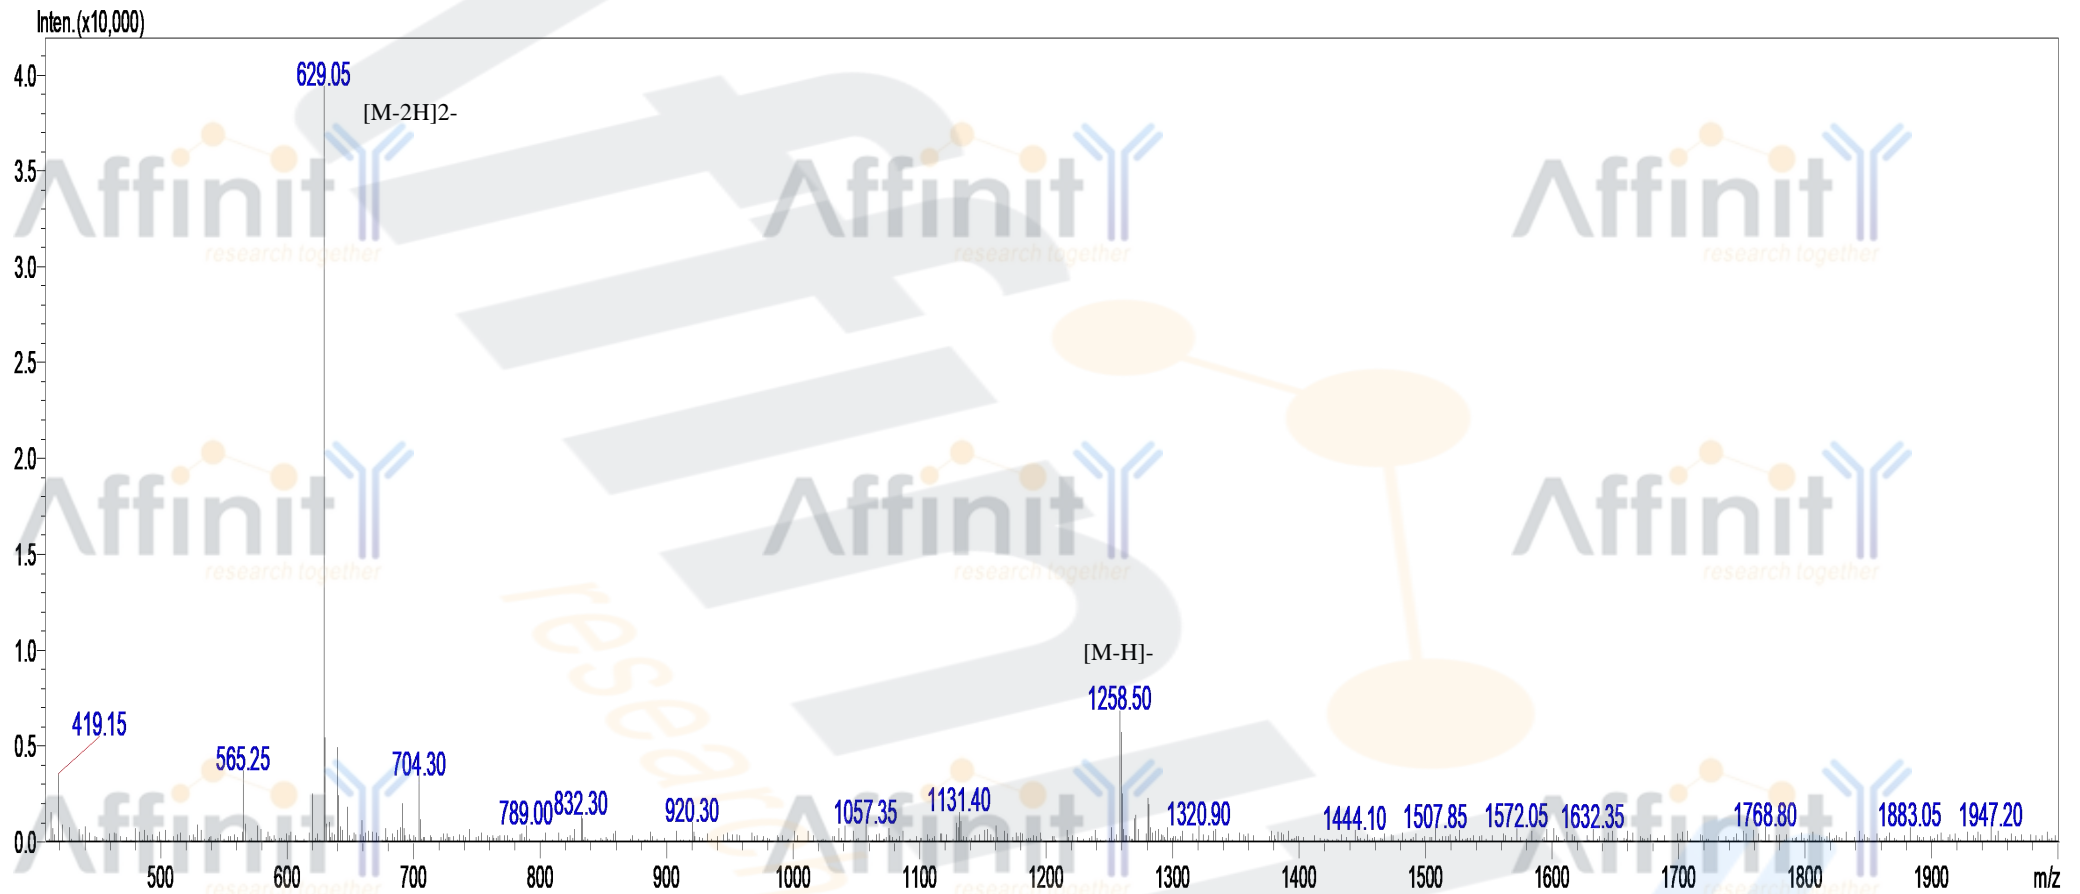

**Sample Description**

Analyzed date: 2014-7-27  
 Analyst: SHAO  
 Sample: E-10P  
 M.W.: 1260.13  
 Lot. No.: P140718-SY594270

**Instrument**

SHIMADZU LCMS-2020  
 Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250°C  
 Block Temp.: 200°C

**Probe Bias:**

+ 4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H2O/50% ACN