


MASS SPECTROMETRY REPORT

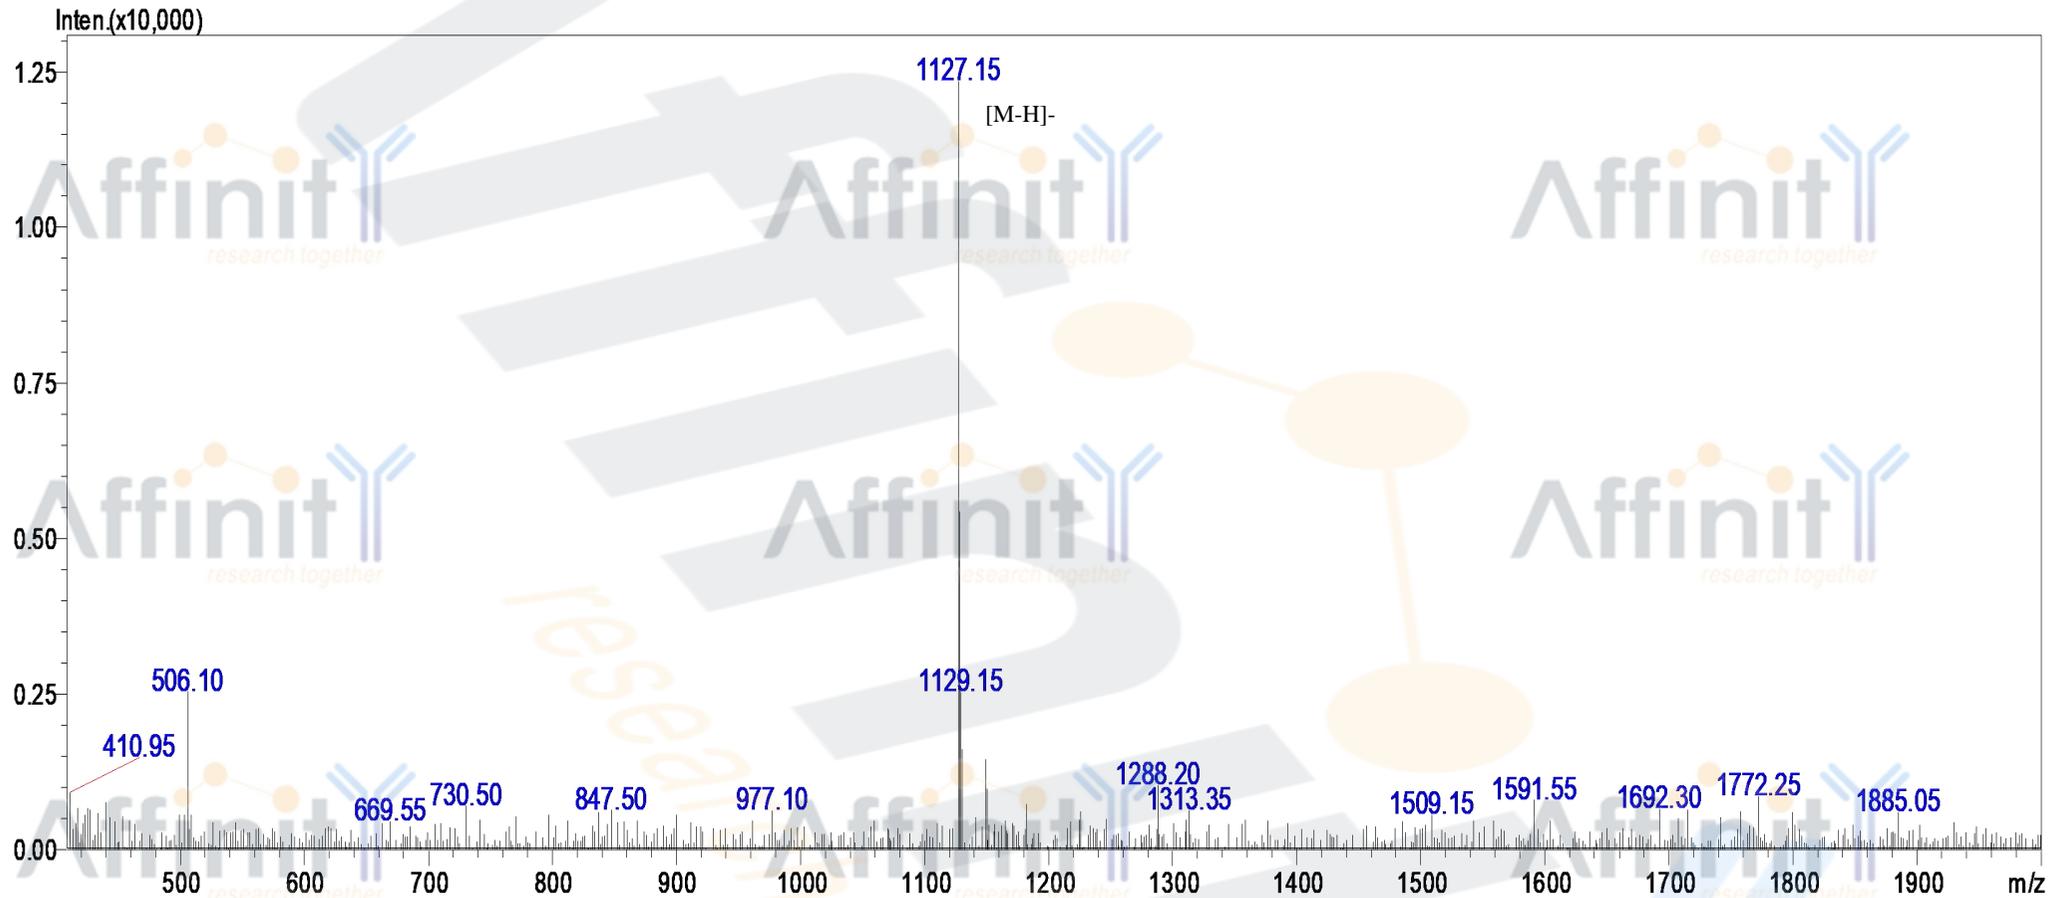

Sample Description

Analyzed date: 2016-6-13
 Analyst: SHAO
 Sample: CC-11
 M.W.: 1129.11
 Lot. No.: P160611-SY659083

Instrument

SHIMADZU LCMS-2020
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp: 250°C
 Block Temp.: 200°C

Probe Bias:

+ 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H₂O/50% ACN