


# MASS SPECTROMETRY REPORT

24-Mar-2017  
12:54:31

Probe: ESI  
Cone: 50v  
Desovation Temp :350  
Capillary:3.00KV  
Extractor: 5v  
Gas Flow : 350  
Scan ES+  
3.20e6

170324-20 130 (2.403) Cm (130:132)

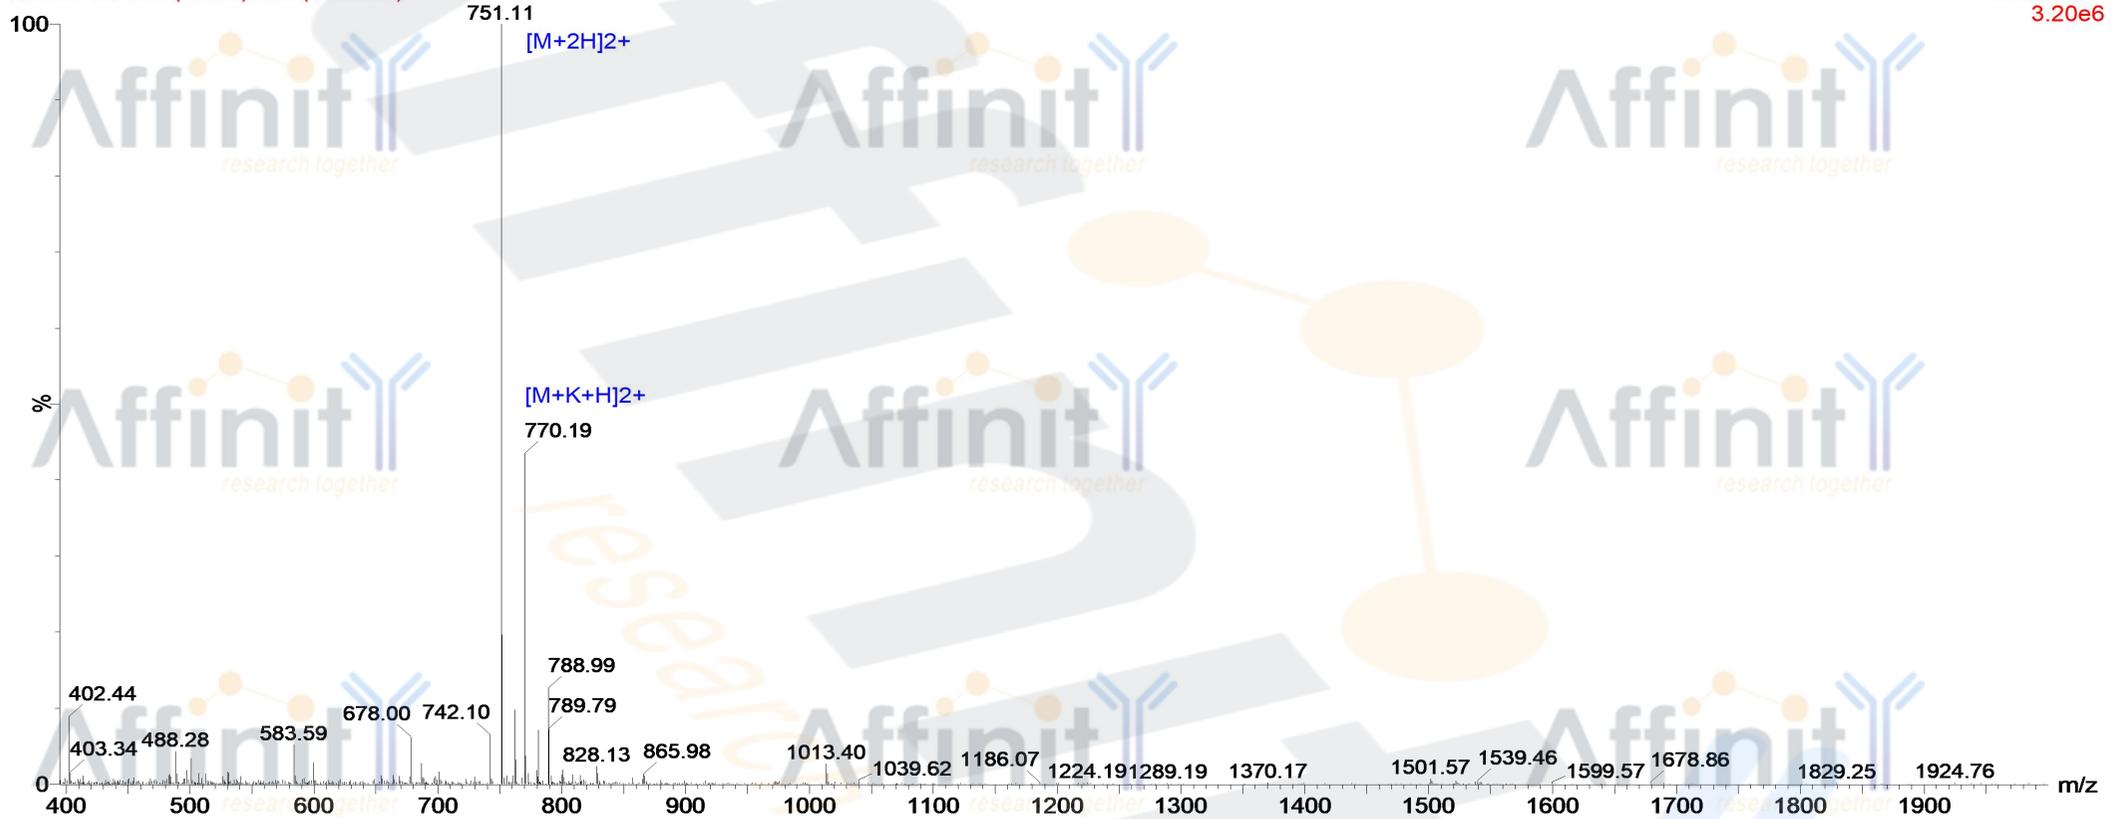

Sample Description

Analyzed date: 2014-03-24  
Analyst: YU  
Sample: K-15  
M.W.: 1499.84  
Lot. No.: P140302-WF328875

Instrument

Waters ZQ2000  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

Probe Bias: + 4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50% H2O/50% ACN