


# MASS SPECTROMETRY REPORT

28-Mar-2017  
13:56:41

Probe: ESI Capillary: 3.00KV  
Cone: 50v Extractor: 5v  
Desolvation Temp: 350 Gas Flow: 350  
Scan ES+  
1.46e7

170328-28 536 (9.907)

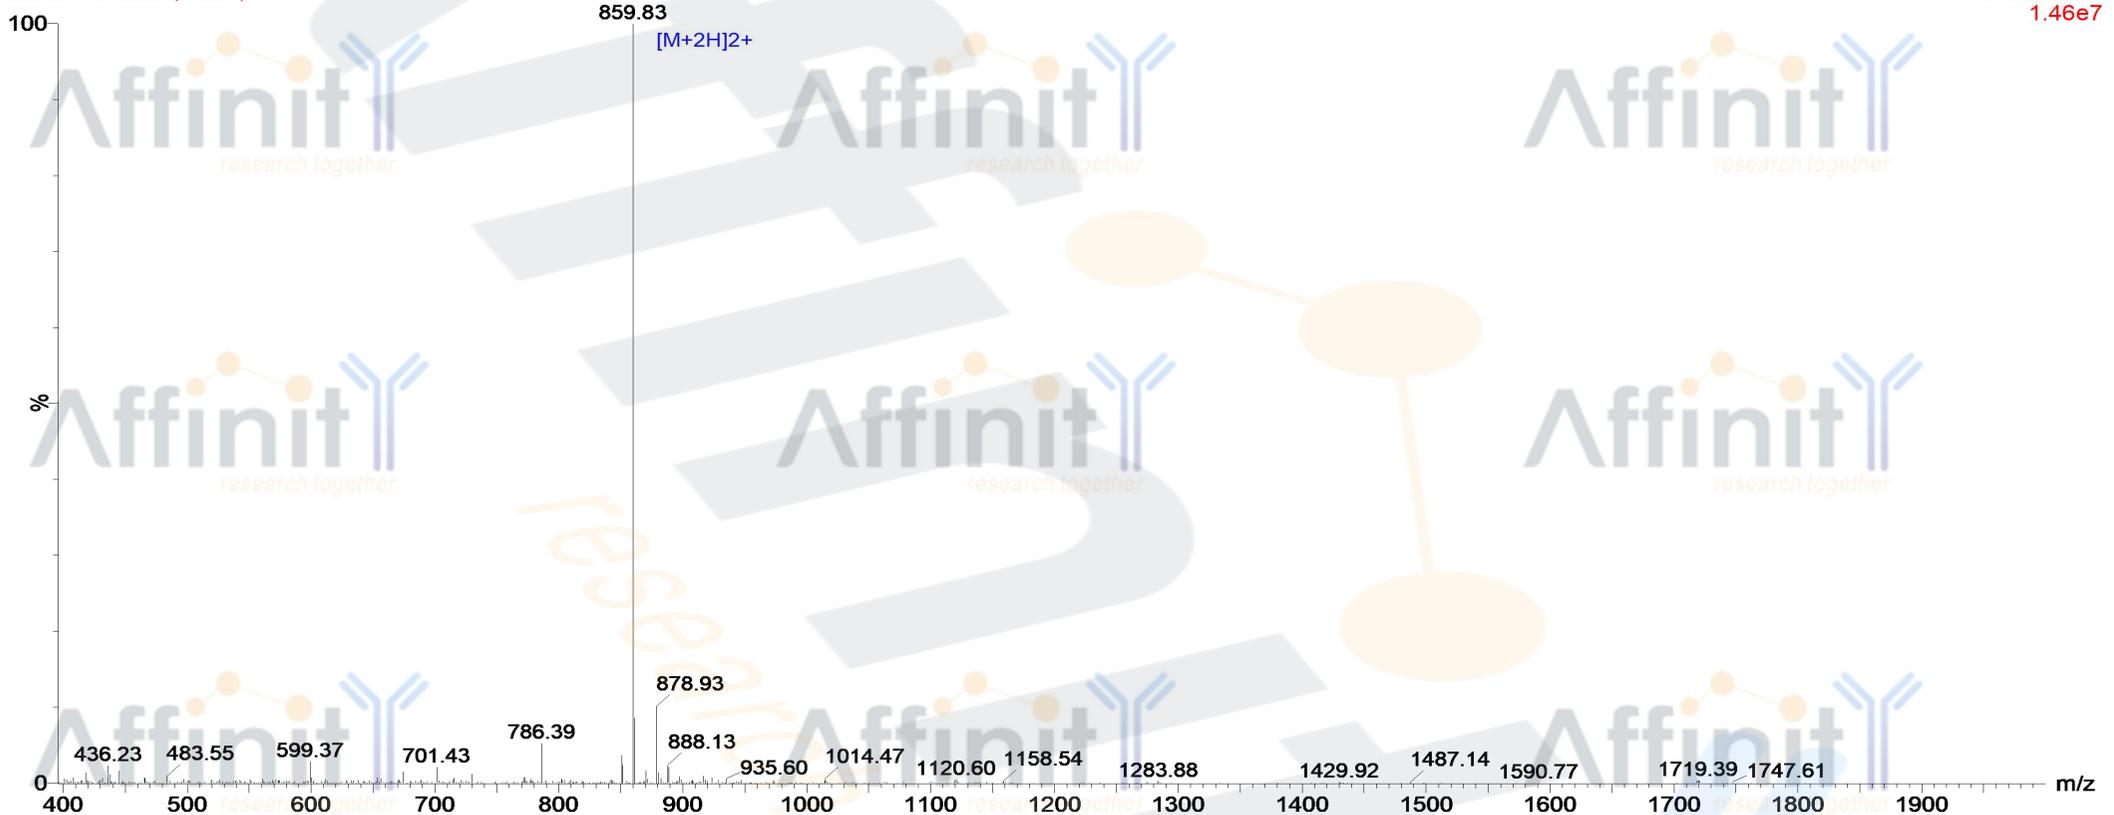

Sample Description

Analyzed date: 2014-03-28  
Analyst: YU  
Sample: Q-15  
M.W.: 1716.89  
Lot. No.: P140302-WF566250

Instrument

Waters ZQ2000  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

Probe Bias: + 4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. Conc.: 50% H2O/50% ACN