


MASS SPECTROMETRY REPORT

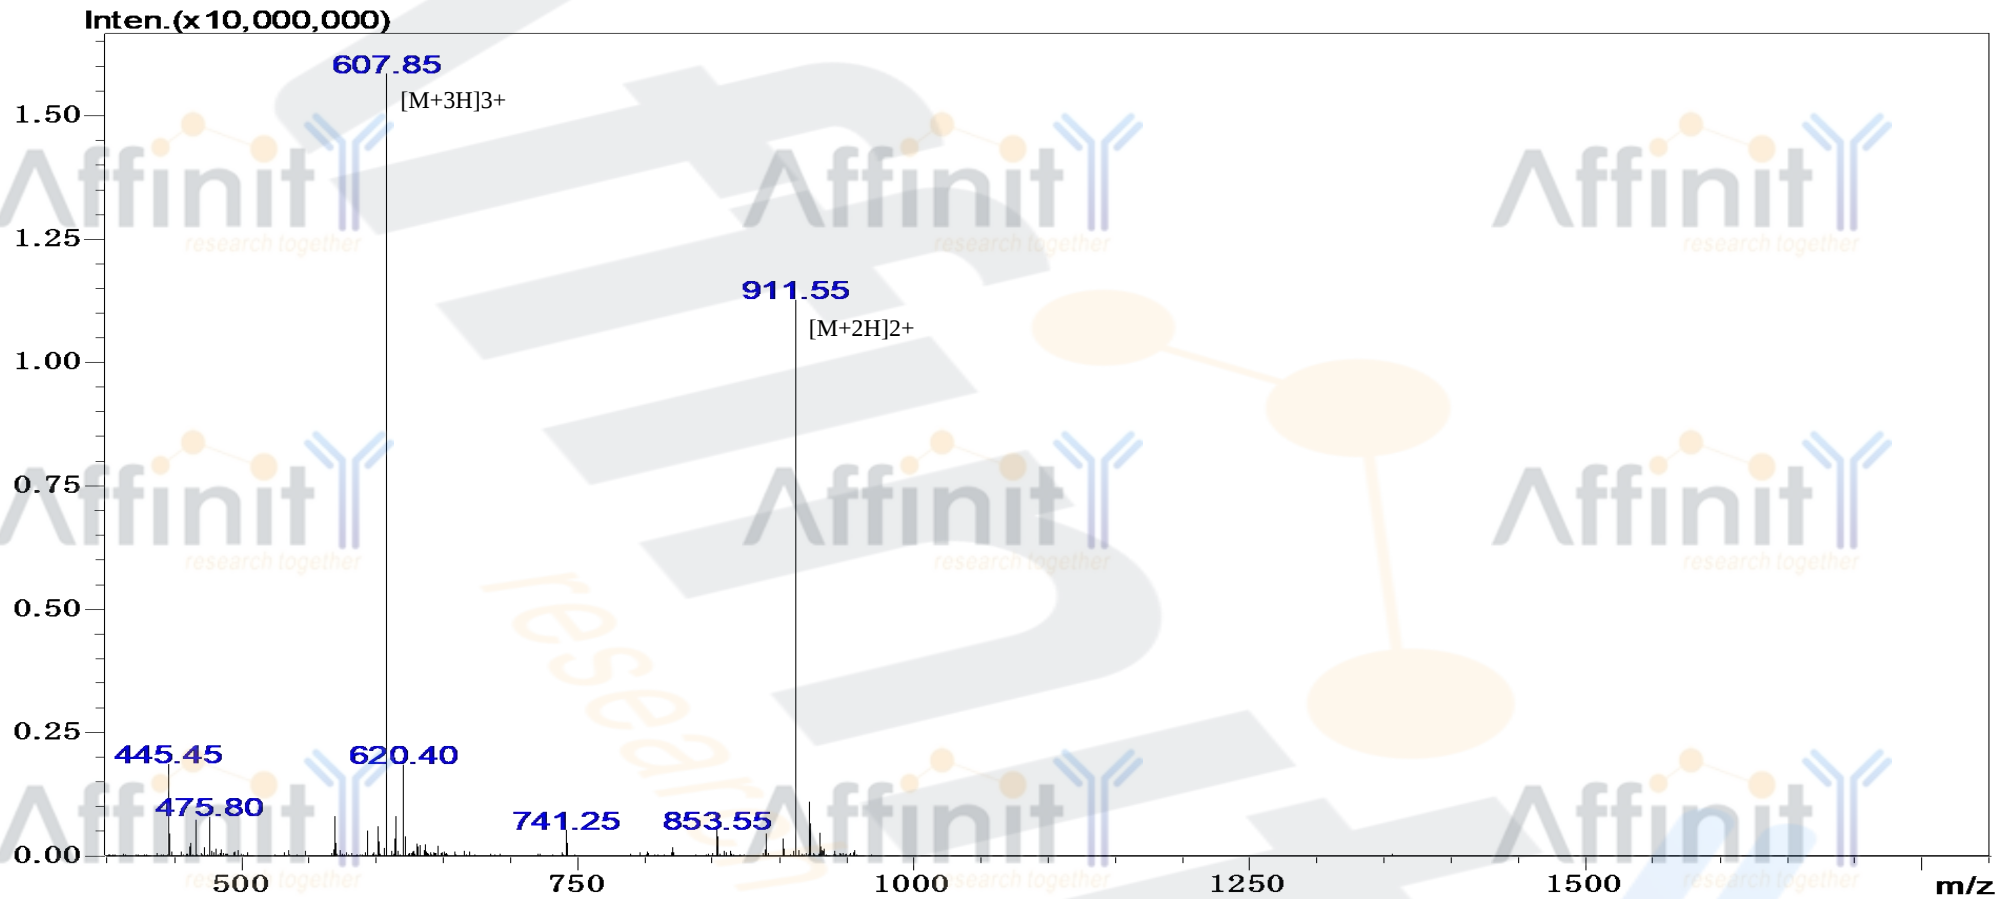

Sample Description

Analyzed date: 2014-7-13
Analyst: Xu
Sample: Y-16
M.W.: 1820.93
Lot. No.: P140705-YS593592

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

SHIMADZU LCMS-2010EV

Probe Bias: + 4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN