


MASS SPECTROMETRY REPORT

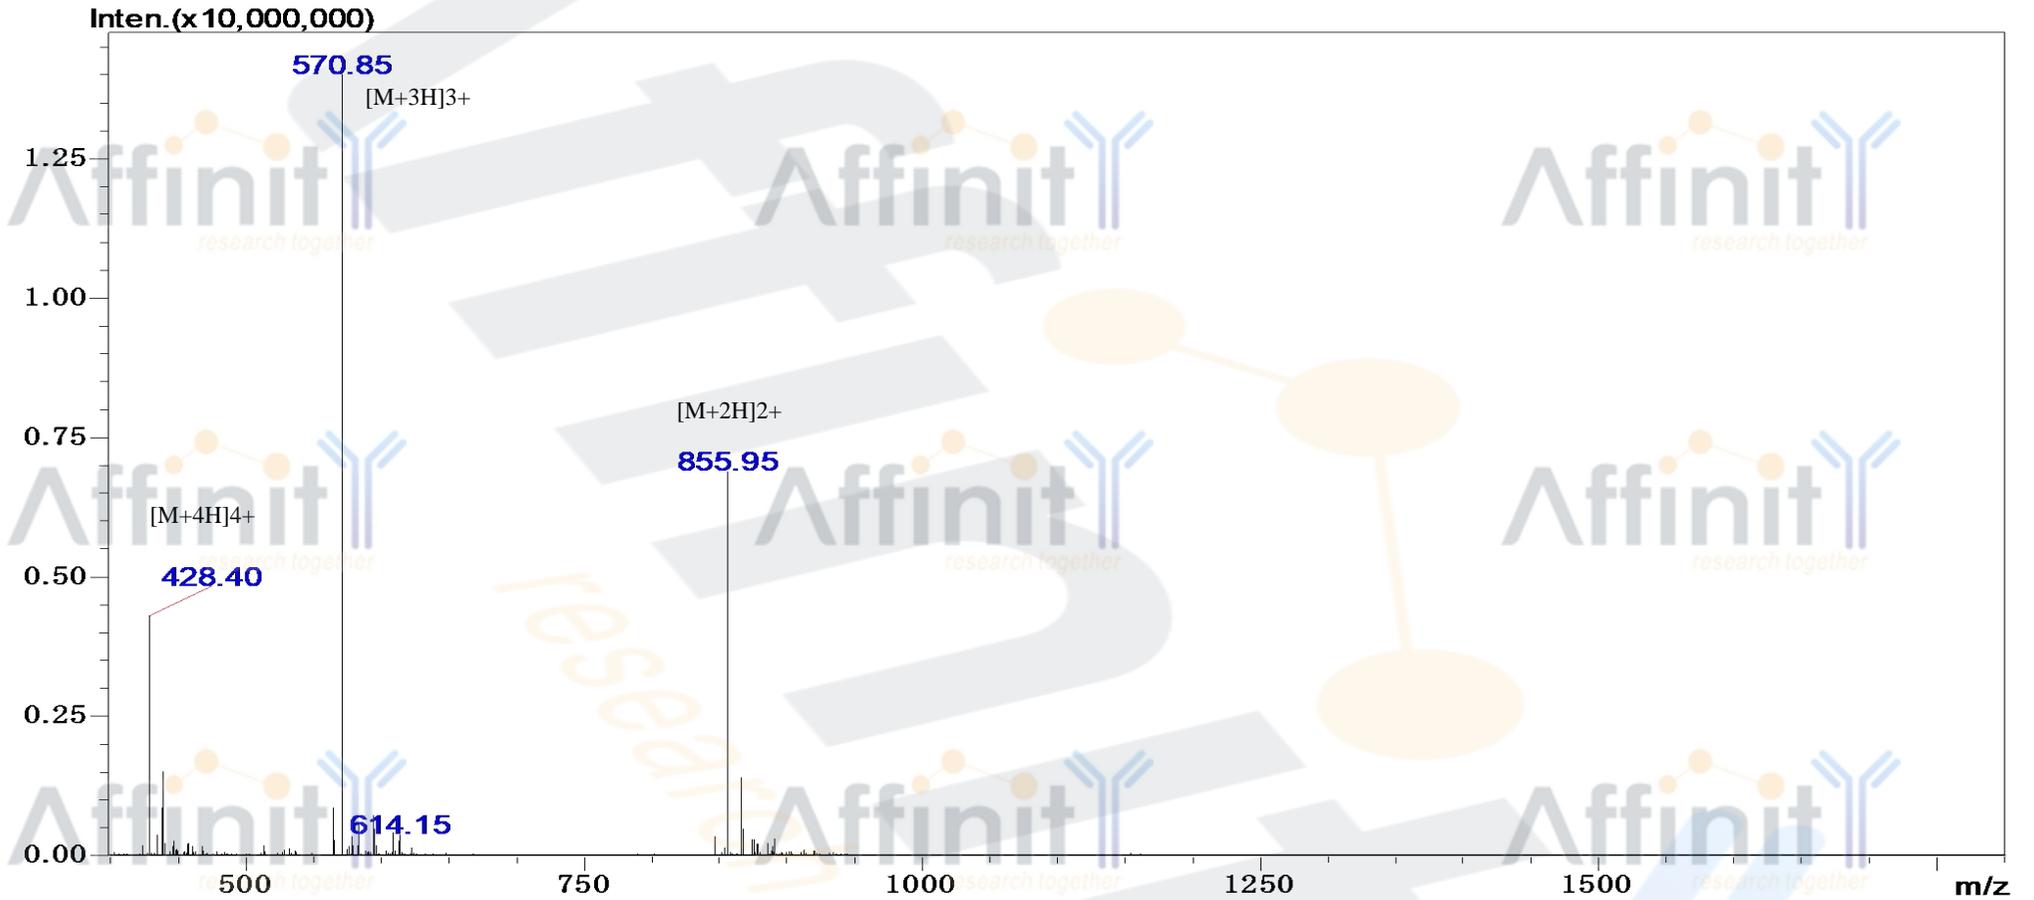

Sample Description

Analyzed date: 2014-7-15
 Analyst: Xu
 Sample: Y-14
 M.W.: 1709.98
 Lot. No.: P140705-YS593620

Instrument

SHIMADZU LCMS-2010EV
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C

Probe Bias:

+ 4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50% H2O/50% ACN