


# MASS SPECTROMETRY REPORT

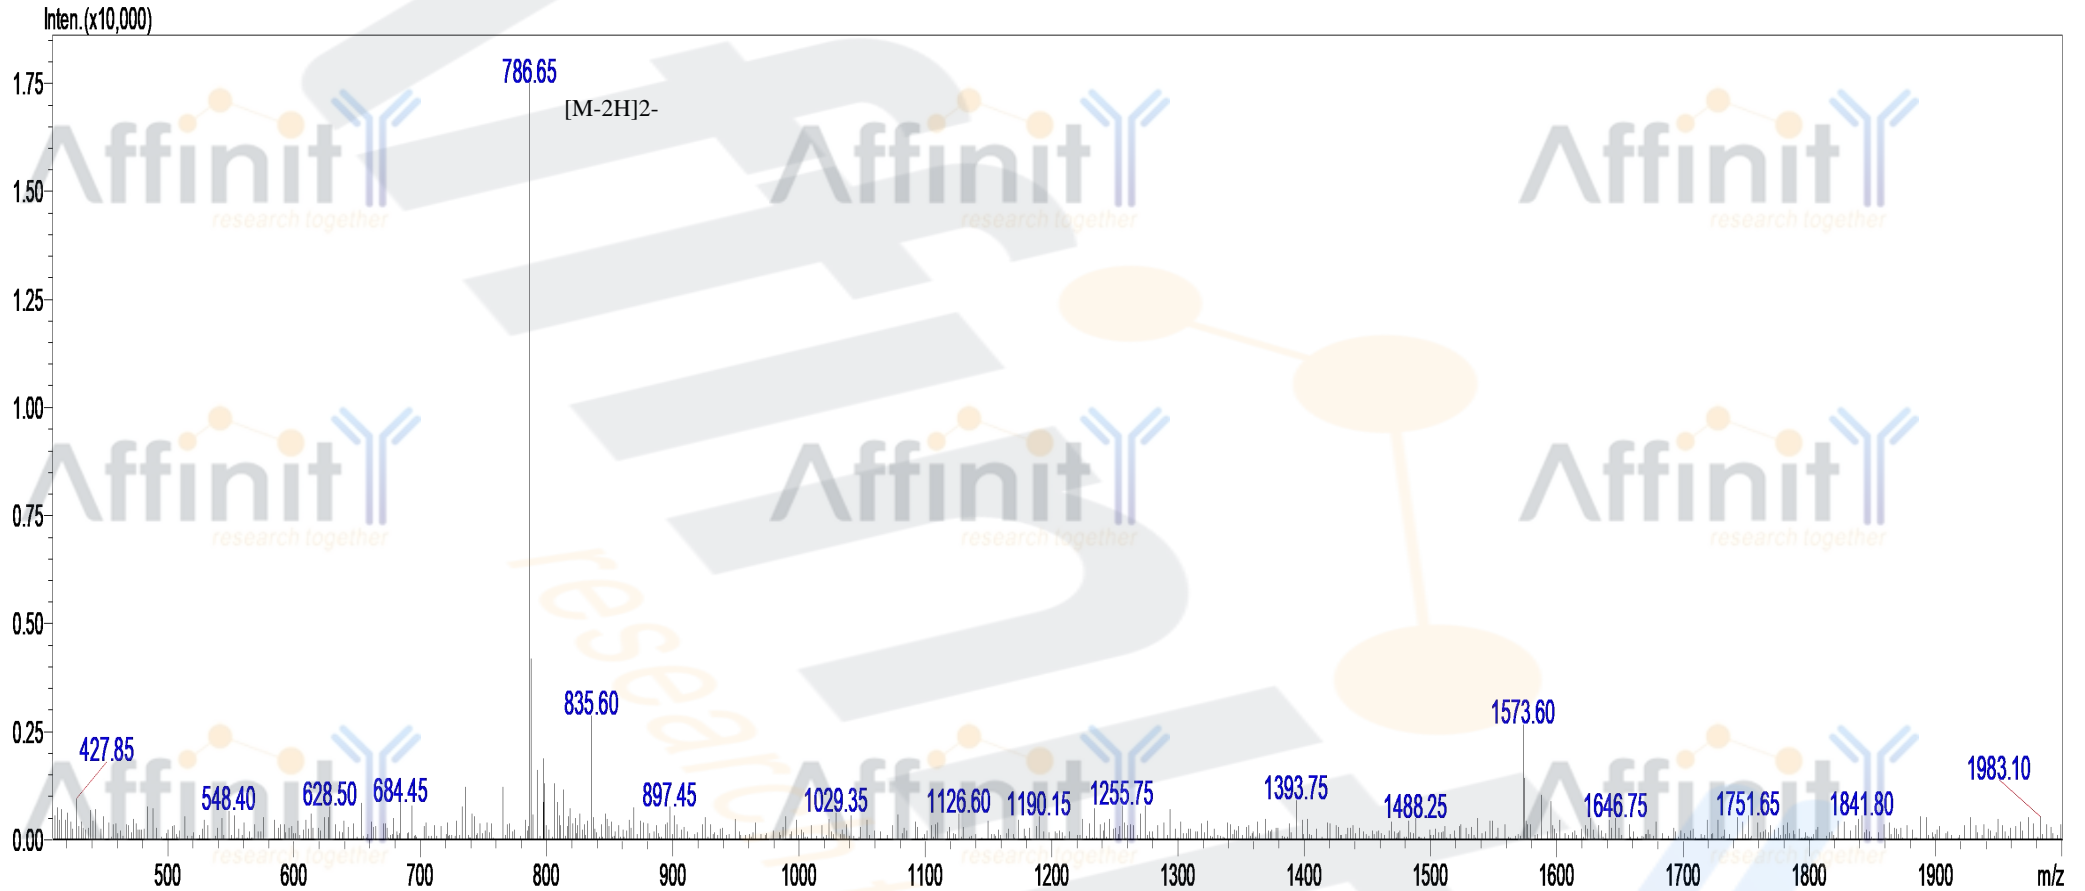

**Sample Description**

Analyzed date: 2014-6-9  
 Analyst: SHAO  
 Sample: N-14  
 M.W.: 1576.72  
 Lot. No.: P140601-HS224870

**Instrument**

SHIMADZU LCMS-2020  
 Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250 °C  
 Block Temp.: 200 °C  
 Probe Bias: + 4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H<sub>2</sub>O/50% ACN