

PAG531Hu01

Polyclonal Antibody to Lysophosphatidylcholine Acyltransferase 3 (LPCAT3)

Organism Species: *Homo sapiens (Human)*

Instruction manual

FOR RESEARCH USE ONLY

NOT FOR USE IN CLINICAL DIAGNOSTIC PROCEDURES

12th Edition (Revised in Aug, 2016)

[PROPERTIES]

Source: Polyclonal antibody preparation

Host: Rabbit

Purification: Antigen-specific affinity chromatography followed by Protein A affinity chromatography

Traits: Liquid

Concentration: 0.48mg/ml

UOM: 100µg(210µl)

Applications: WB; IHC; ICC; IP.

[IMMUNOGEN]

Immunogen: Recombinant LPCAT3 (Met122~Arg233) expressed in *E.coli*

Accession No.: RPG531Hu01

[APPLICATIONS]

Western blotting: 0.5-2µg/mL;1:240-960

Immunohistochemistry: 5-20µg/mL;1:24-96

Immunocytochemistry: 5-20µg/mL;1:24-96

Optimal working dilutions must be determined by end user.

[FORMULATION]

Form & Buffer: Supplied as solution form in PBS, pH7.4, containing 0.02% NaN₃, 50% glycerol.

[STORAGE AND STABILITY]

Storage: Avoid repeated freeze/thaw cycles.

Store at 4°C for frequent use.

Aliquot and store at -20°C for 12 months.

Stability Test: The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the

expiration date under appropriate storage condition.

[IDENTIFICATION]

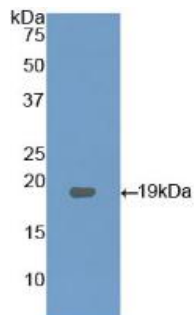


Figure. Western Blot; Sample: Recombinant LPCAT3, Human.

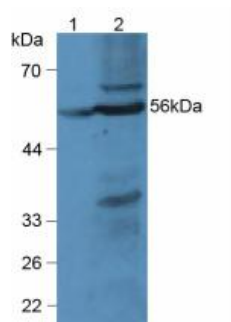


Figure. Western Blot; Sample: Lane1: Rat Liver Tissue; Lane2: Mouse Liver Tissue.

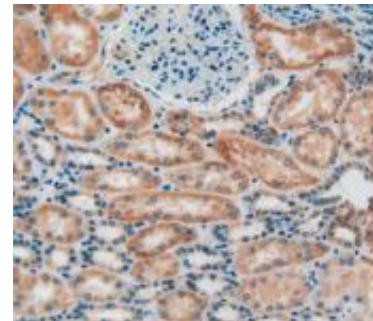


Figure. DAB staining on IHC-P; Samples: Human Kidney Tissue.

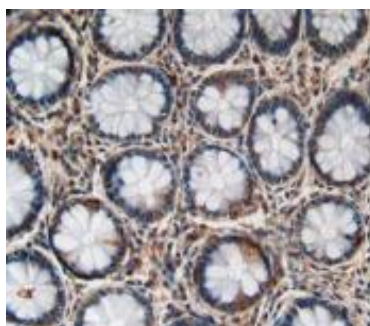


Figure. DAB staining on IHC-P; Samples: Human Rectum Tissue.

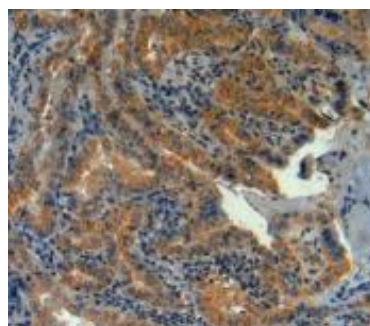


Figure. DAB staining on IHC-P; Samples: Human Thyroid Cancer Tissue.

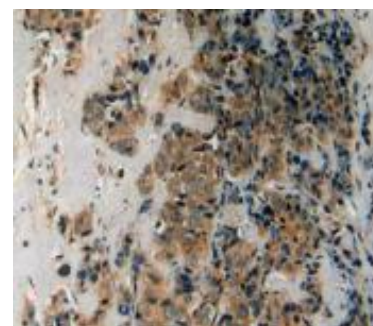


Figure. DAB staining on IHC-P; Samples: Human Breast Cancer Tissue.

[IMPORTANT NOTE]

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.